

LB103421


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

44771

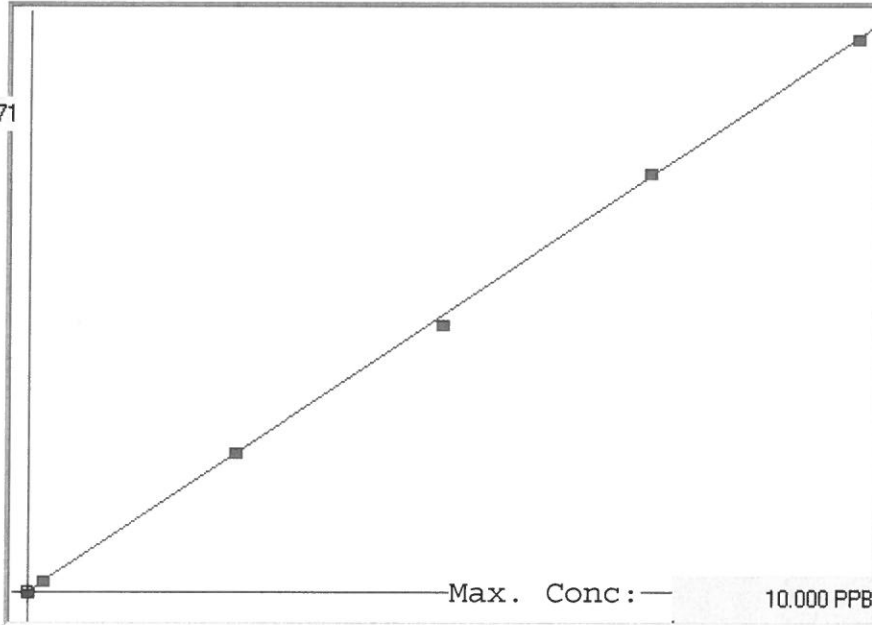

A= 0.0000e+000

B= 2.2328e-004

C= 2.7973e-004

Rho= 0.9997978

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.007	0.007	31	0.000	31				
0.2	0.200	0.213	0.013	953	0.0 %	953				
2.5	2.500	2.551	0.051	11425	0.0 %	11425				
5.0	5.000	4.848	-0.152	21710	0.0 %	21710				
7.5	7.500	7.584	0.084	33963	0.0 %	33963				
10.0	10.000	9.997	-0.003	44771	0.0 %	44771				

LB103421 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 14 Jun 2019 15:04:26

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50.0	31	-	0.00007470A	PPB	14 Jun 2019 15:04:40	S	Std
0.2 - 1	50.2	953	-	0.20007470A	PPB	14 Jun 2019 15:06:49	S	Std
2.5 - 1	52.5	11425	-	2.50007470A	PPB	14 Jun 2019 15:08:57	S	Std
5.0 - 1	55.0	21710	-	5.00007470A	PPB	14 Jun 2019 15:11:06	S	Std
7.5 - 1	57.5	33963	-	7.50007470A	PPB	14 Jun 2019 15:13:14	S	Std
10.0 - 1	510.0	44771	-	10.00007470A	PPB	14 Jun 2019 15:20:53	S	Std
ICV96 - 1	ICV96	17997	4.0187	-7470A	PPB	14 Jun 2019 15:26:20	U	SMPL
ICB96 - 1	ICB96	-29	-0.0062	-7470A	PPB	14 Jun 2019 15:28:27	U	SMPL
CCV71 - 1	CCV71	21825	4.8735	-7470A	PPB	14 Jun 2019 15:30:34	U	SMPL
CCB71 - 1	CCB71	-47	-0.0102	-7470A	PPB	14 Jun 2019 15:32:40	U	SMPL
CRA - 1	CRA	956	0.2137	-7470A	PPB	14 Jun 2019 15:34:49	U	SMPL
HighStd - 1	HighStd	44807	10.0050	-7470A	PPB	14 Jun 2019 15:36:55	U	SMPL
ChkStd - 1	ChkStd	31982	7.1414	-7470A	PPB	14 Jun 2019 15:39:02	U	SMPL
PB120629BL - 1	PBW	-30	-0.0064	-7470A	PPB	14 Jun 2019 15:41:10	U	SMPL
PB120629BS - 1	LCSW	17739	3.9611	-7470A	PPB	14 Jun 2019 15:43:18	U	SMPL
K3156-04 - 1	HD-01-061219	-96	-0.0212	-7470A	PPB	14 Jun 2019 15:45:25	U	SMPL
K3156-04DUP - 1	HD-01-061219DUP	-49	-0.0107	-7470A	PPB	14 Jun 2019 15:47:33	U	SMPL
K3156-04MS - 1	HD-01-061219MS	18361	4.1000	-7470A	PPB	14 Jun 2019 15:49:42	U	SMPL
K3156-04MSD - 1	HD-01-061219MSD	18349	4.0973	-7470A	PPB	14 Jun 2019 15:51:51	U	SMPL
K3351-02 - 1	RT-3407	-94	-0.0207	-7470A	PPB	14 Jun 2019 15:53:57	U	SMPL
CCV72 - 1	CCV72	22002	4.9130	-7470A	PPB	14 Jun 2019 15:56:03	U	SMPL
CCB72 - 1	CCB72	-43	-0.0093	-7470A	PPB	14 Jun 2019 15:58:10	U	SMPL
K3351-04 - 1	RT-3425	-20	-0.0042	-7470A	PPB	14 Jun 2019 16:00:18	U	SMPL
K3351-06 - 1	RBR-200029	-26	-0.0055	-7470A	PPB	14 Jun 2019 16:02:25	U	SMPL
K3351-08 - 1	RT-3860	-34	-0.0073	-7470A	PPB	14 Jun 2019 16:04:34	U	SMPL
K3352-02 - 1	20190612-LOC-11	-42	-0.0091	-7470A	PPB	14 Jun 2019 16:06:44	U	SMPL
K3352-04 - 1	20190612-LOC-12	-6	-0.0011	-7470A	PPB	14 Jun 2019 16:08:51	U	SMPL
K3368-01 - 1	SOIL	-33	-0.0071	-7470A	PPB	14 Jun 2019 16:10:58	U	SMPL
K3369-07 - 1	Z-3-SOIL-1	-38	-0.0082	-7470A	PPB	14 Jun 2019 16:13:07	U	SMPL
K3369-11 - 1	Z-3-SOIL-2	-26	-0.0055	-7470A	PPB	14 Jun 2019 16:15:15	U	SMPL
K3369-15 - 1	Z-3-SOIL-3	-33	-0.0071	-7470A	PPB	14 Jun 2019 16:17:23	U	SMPL
K3369-19 - 1	Z-3-SOIL-4	-26	-0.0055	-7470A	PPB	14 Jun 2019 16:19:30	U	SMPL
CCV73 - 1	CCV73	21869	4.8833	-7470A	PPB	14 Jun 2019 16:21:37	U	SMPL
CCB73 - 1	CCB73	-67	-0.0147	-7470A	PPB	14 Jun 2019 16:23:44	U	SMPL
K3370-01 - 1	OIL-WATER-SEPERATOR(OWS)-1	-33	-0.0071	-7470A	PPB	14 Jun 2019 16:25:51	U	SMPL
PB120630BL - 1	PBW	79	0.0179	-7470A	PPB	14 Jun 2019 16:27:57	U	SMPL
PB120630BS - 1	LCSW	17747	3.9629	-7470A	PPB	14 Jun 2019 16:30:04	U	SMPL
K3294-05 - 1	W1	7166	1.6003	-7470A	PPB	14 Jun 2019 16:32:11	U	SMPL
K3294-06 - 1	W2	2216	0.4951	-7470A	PPB	14 Jun 2019 16:34:18	U	SMPL
K3369-01 - 1	FRAC-TANK-COMP	196	0.0440	-7470A	PPB	14 Jun 2019 16:36:26	U	SMPL
K3372-01 - 1	EFFL-B2-79	1935	0.4323	-7470A	PPB	14 Jun 2019 16:38:33	U	SMPL
K3373-01 - 1	13857-13964-13981	1268	0.2834	-7470A	PPB	14 Jun 2019 16:40:42	U	SMPL
K3373-01DUP - 1	13857-13964-13981DUP	1107	0.2475	-7470A	PPB	14 Jun 2019 16:42:50	U	SMPL
K3373-01MS - 1	13857-13964-13981MS	17364	3.8774	-7470A	PPB	14 Jun 2019 16:44:57	U	SMPL
CCV74 - 1	CCV74	21594	4.8219	-7470A	PPB	14 Jun 2019 16:47:03	U	SMPL
CCB74 - 1	CCB74	-100	-0.0220	-7470A	PPB	14 Jun 2019 16:49:12	U	SMPL
K3373-01MSD - 1	13857-13964-13981MSD	18529	4.1375	-7470A	PPB	14 Jun 2019 16:51:26	U	SMPL
PB120629TB - 1	PB120582TB	-150	-0.0332	-7470A	PPB	14 Jun 2019 16:53:36	U	SMPL
K3156-04LX5 - 1		-164	-0.0363	-7470A	PPB	14 Jun 2019 16:55:43	U	SMPL
K3156-04A - 1		18227	4.0701	-7470A	PPB	14 Jun 2019 16:57:50	U	SMPL
K3373-01LX5 - 1		133	0.0300	-7470A	PPB	14 Jun 2019 16:59:57	U	SMPL
K3373-01A - 1		18464	4.1230	-7470A	PPB	14 Jun 2019 17:02:05	U	SMPL
CCV75 - 1	CCV75	21806	4.8692	-7470A	PPB	14 Jun 2019 17:04:13	U	SMPL
CCB75 - 1	CCB75	-79	-0.0174	-7470A	PPB	14 Jun 2019 17:06:21	U	SMPL