

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/14/2019 15:16

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.093	0.0	0.104	
ICB1	-0.141	0.0	0.004	
CCV1	241.007	0.0	0.253	
CCB1	-0.320	0.0	0.004	
PB120620BL	-0.596	0.0	0.004	
PB120620BS	97.599	0.0	0.105	
LOWPB120620	9.251	0.0	0.014	
HIGHPB120620	488.595	0.0	0.509	
K3351-01	0.020	0.0	0.004	
K3351-01DUP	-0.344	0.0	0.004	
K3351-01MS	31.100	0.0	0.036	
K3351-01MSD	30.633	0.0	0.036	
K3351-03	-0.174	0.0	0.004	
K3351-05	0.137	0.0	0.004	
CCV2	242.335	0.0	0.255	
CCB2	-0.332	0.0	0.004	
K3351-07	-0.215	0.0	0.004	
K3361-02	-0.522	0.0	0.004	
K3361-04	9.870	0.0	0.015	
K3369-04	-0.386	0.0	0.004	
K3369-08	-0.150	0.0	0.004	
K3369-12	-0.077	0.0	0.004	
K3369-16	0.279	0.0	0.005	
PB120621BL	-0.369	0.0	0.004	
PB120621BS	96.547	0.0	0.104	
K3369-01	2.103	0.0	0.006	
CCV3	242.433	0.0	0.255	
CCB3	-0.273	0.0	0.004	
K3369-01DUP	1.854	0.0	0.006	
K3369-01MS	35.886	0.0	0.041	
K3369-01MSD	36.092	0.0	0.042	
K3366-01	0.297	0.0	0.005	
CCV4	252.358	0.0	0.265	
CCB4	-0.208	0.0	0.004	

N 34
Mean 56.188
SD 110.5665
CV% 196.78

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/14/2019 10:40

Test Total CN


Accepted 6/14/2019 10:40

Factor 967.3

Bias 0.004

Coeff. of det. 0.999939

Errors

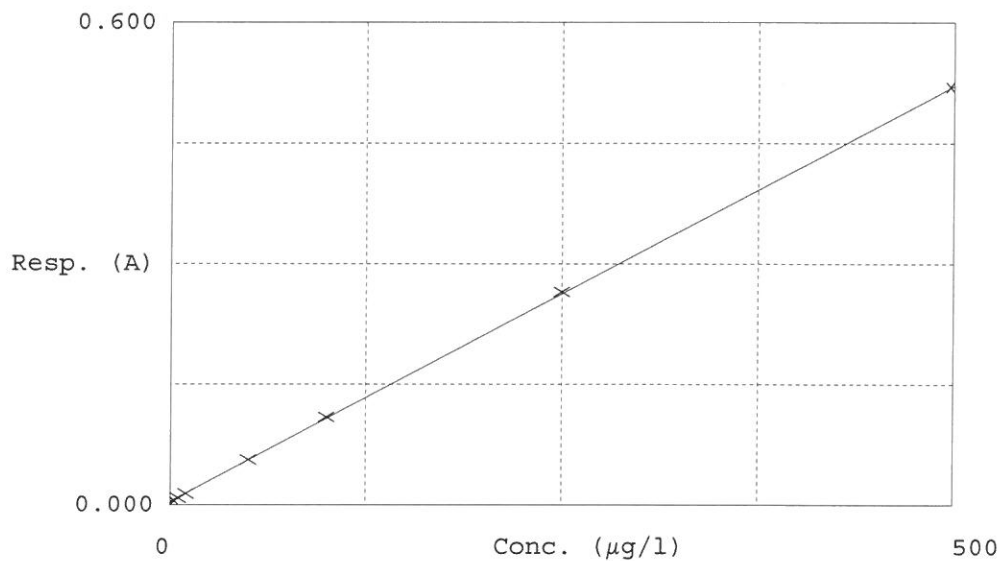

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.8884	0.0000	
2	5.0PPBCN	0.008	4.0109	5.0000	
3	10PPBCN	0.014	9.2674	10.0000	
4	50PPBCN	0.056	50.1716	50.0000	
5	100PPBCN	0.109	101.5714	100.0000	
6	250PPBCN	0.265	252.3479	250.0000	
7	500PPBCN	0.520	498.5192	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Fri Jun 14 14:55:20 2019

Fri Jun 14 15:15:47 2019

AS

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.8884	µg/l	6/14/2019 10:40:07	
5.OPPBCN	A	Total CN	P	4.0109	µg/l	6/14/2019 10:40:08	
10PPBCN	A	Total CN	P	9.2674	µg/l	6/14/2019 10:40:09	
50PPBCN	A	Total CN	P	50.1716	µg/l	6/14/2019 10:40:10	
100PPBCN	A	Total CN	P	101.5714	µg/l	6/14/2019 10:40:11	
250PPBCN	A	Total CN	P	252.3479	µg/l	6/14/2019 10:40:12	
500PPBCN	A	Total CN	P	498.5192	µg/l	6/14/2019 10:40:13	
ICV1	S	Total CN	P	96.0927	µg/l	6/14/2019 14:55:20	
ICB1	S	Total CN	P	-0.1412	µg/l	6/14/2019 14:55:21	
CCV1	S	Total CN	P	241.0074	µg/l	6/14/2019 14:55:22	
CCB1	S	Total CN	P	-0.3203	µg/l	6/14/2019 14:55:23	
PB120620BL	S	Total CN	P	-0.596	µg/l	6/14/2019 14:55:24	
PB120620BS	S	Total CN	P	97.5992	µg/l	6/14/2019 14:55:25	
LOWPB120620	S	Total CN	P	9.2507	µg/l	6/14/2019 14:55:26	
HIGHPB120620	S	Total CN	P	488.5947	µg/l	6/14/2019 14:55:27	
K3351-01	S	Total CN	P	0.0196	µg/l	6/14/2019 14:55:28	
K3351-01DUP	S	Total CN	P	-0.3435	µg/l	6/14/2019 14:55:29	
K3351-01MS	S	Total CN	P	31.0998	µg/l	6/14/2019 14:55:30	
K3351-01MSD	S	Total CN	P	30.6332	µg/l	6/14/2019 15:02:55	
K3351-03	S	Total CN	P	-0.174	µg/l	6/14/2019 15:02:56	
K3351-05	S	Total CN	P	0.137	µg/l	6/14/2019 15:02:57	
CCV2	S	Total CN	P	242.3349	µg/l	6/14/2019 15:02:58	
CCB2	S	Total CN	P	-0.3318	µg/l	6/14/2019 15:02:59	
K3351-07	S	Total CN	P	-0.2152	µg/l	6/14/2019 15:03:00	
K3361-02	S	Total CN	P	-0.5216	µg/l	6/14/2019 15:03:01	
K3361-04	S	Total CN	P	9.8699	µg/l	6/14/2019 15:03:02	
K3369-04	S	Total CN	P	-0.386	µg/l	6/14/2019 15:03:03	
K3369-08	S	Total CN	P	-0.1497	µg/l	6/14/2019 15:03:04	
K3369-12	S	Total CN	P	-0.0766	µg/l	6/14/2019 15:03:05	
K3369-16	S	Total CN	P	0.2791	µg/l	6/14/2019 15:10:27	
PB120621BL	S	Total CN	P	-0.3689	µg/l	6/14/2019 15:10:28	
PB120621BS	S	Total CN	P	96.547	µg/l	6/14/2019 15:10:29	
K3369-01	S	Total CN	P	2.1026	µg/l	6/14/2019 15:10:30	
CCV3	S	Total CN	P	242.4332	µg/l	6/14/2019 15:10:31	
CCB3	S	Total CN	P	-0.2726	µg/l	6/14/2019 15:10:32	
K3369-01DUP	S	Total CN	P	1.8541	µg/l	6/14/2019 15:10:33	
K3369-01MS	S	Total CN	P	35.8855	µg/l	6/14/2019 15:10:34	
K3369-01MSD	S	Total CN	P	36.092	µg/l	6/14/2019 15:10:35	
K3366-01	S	Total CN	P	0.2967	µg/l	6/14/2019 15:10:36	
CCV4	S	Total CN	P	252.3576	µg/l	6/14/2019 15:15:45	
CCB4	S	Total CN	P	-0.2079	µg/l	6/14/2019 15:15:46	