


LB103472

7471B

INSTRUMENT ID : CU1

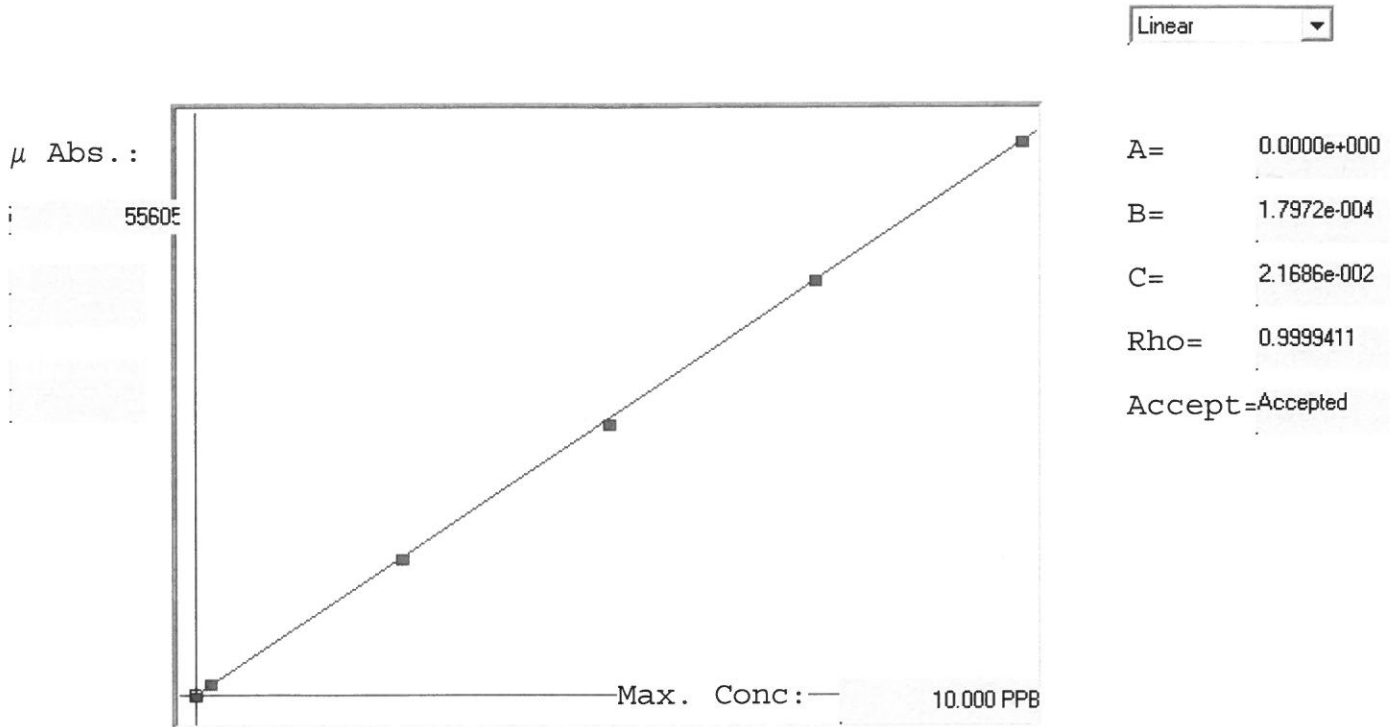

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.001	0.001	-113	0.000	-113				
0.2	0.200	0.230	0.030	1159	0.0 %	1159				
2.5	2.500	2.506	0.006	13826	0.0 %	13826				
5.0	5.000	4.914	-0.086	27223	0.0 %	27223				
7.5	7.500	7.533	0.033	41795	0.0 %	41795				
10.0	10.000	10.015	0.015	55605	0.0 %	55605				

LB103472 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 18 Jun 2019 12:53:51				
Sample ID	Extended ID	μ Abs.	Conc.	Std. Conc	Method	Units	Date	Type
0.0 - 1	50.0	-113	-	0.0000	7471B	PPB	18 Jun 2019 12:54:54	S Std
0.2 - 1	50.2	1159	-	0.2000	7471B	PPB	18 Jun 2019 12:57:11	S Std
2.5 - 1	52.5	13826	-	2.5000	7471B	PPB	18 Jun 2019 12:59:29	S Std
5.0 - 1	55.0	27223	-	5.0000	7471B	PPB	18 Jun 2019 13:01:46	S Std
7.5 - 1	57.5	41795	-	7.5000	7471B	PPB	18 Jun 2019 13:04:03	S Std
10.0 - 1	510.0	55605	-	10.0000	7471B	PPB	18 Jun 2019 13:06:20	S Std
ICV100 - 1	ICV100	21947	3.9660	-	7471B	PPB	18 Jun 2019 13:10:22	U SMPL
ICB100 - 1	ICB100	-201	-0.0144	-	7471B	PPB	18 Jun 2019 13:12:38	U SMPL
CCV85 - 1	CCV85	26825	4.8426	-	7471B	PPB	18 Jun 2019 13:14:54	U SMPL
CCB85 - 1	CCB85	-185	-0.0116	-	7471B	PPB	18 Jun 2019 13:17:09	U SMPL
CRA - 1	CRA	1159	0.2300	-	7471B	PPB	18 Jun 2019 13:19:26	U SMPL
HighStd - 1	HighStd	54465	9.8101	-	7471B	PPB	18 Jun 2019 13:21:42	U SMPL
ChkStd - 1	ChkStd	38603	6.9594	-	7471B	PPB	18 Jun 2019 13:23:57	U SMPL
PB120715BL - 1	PBS	-184	-0.0114	-	7471B	PPB	18 Jun 2019 13:26:15	U SMPL
PB120715BS - 1	LCSS	20142	3.6416	-	7471B	PPB	18 Jun 2019 13:28:33	U SMPL
K3121-01 - 1	WASTE	862	0.1766	-	7471B	PPB	18 Jun 2019 13:30:50	U SMPL
K3157-01 - 1	CL-01-061719-A	3450	0.6417	-	7471B	PPB	18 Jun 2019 13:33:07	U SMPL
K3157-03 - 1	CL-01-061719-B	2446	0.4613	-	7471B	PPB	18 Jun 2019 13:35:24	U SMPL
K3157-05 - 1	CL-01-061719-C	3100	0.5788	-	7471B	PPB	18 Jun 2019 13:37:42	U SMPL
K3157-07 - 1	CL-01-061719-D	1672	0.3222	-	7471B	PPB	18 Jun 2019 13:39:58	U SMPL
CCV86 - 1	CCV86	26782	4.8349	-	7471B	PPB	18 Jun 2019 13:42:14	U SMPL
CCB86 - 1	CCB86	-190	-0.0125	-	7471B	PPB	18 Jun 2019 13:44:29	U SMPL
K3157-09 - 1	CL-01-061719-E	6189	1.1340	-	7471B	PPB	18 Jun 2019 13:46:46	U SMPL
K3158-03 - 1	OK-01-061719	829	0.1707	-	7471B	PPB	18 Jun 2019 13:49:02	U SMPL
K3419-01 - 1	TP-A	461	0.1045	-	7471B	PPB	18 Jun 2019 13:51:18	U SMPL
K3419-03 - 1	TP-B	1281	0.2519	-	7471B	PPB	18 Jun 2019 13:53:35	U SMPL
K3419-05 - 1	TP-C	612	0.1317	-	7471B	PPB	18 Jun 2019 13:55:51	U SMPL
K3419-07 - 1	TP-D	180	0.0540	-	7471B	PPB	18 Jun 2019 13:58:08	U SMPL
K3419-09 - 1	TP-E	174	0.0530	-	7471B	PPB	18 Jun 2019 14:00:25	U SMPL
K3420-02 - 1	BAT-B12	580	0.1259	-	7471B	PPB	18 Jun 2019 14:02:42	U SMPL
K3420-02DUP - 1	BAT-B12DUP	580	0.1259	-	7471B	PPB	18 Jun 2019 14:04:59	U SMPL
K3420-02MS - 1	BAT-B12MS	21281	3.8463	-	7471B	PPB	18 Jun 2019 14:07:15	U SMPL
CCV87 - 1	CCV87	27134	4.8982	-	7471B	PPB	18 Jun 2019 14:09:31	U SMPL
CCB87 - 1	CCB87	-161	-0.0072	-	7471B	PPB	18 Jun 2019 14:11:47	U SMPL
K3420-02MSD - 1	BAT-B12MSD	21426	3.8723	-	7471B	PPB	18 Jun 2019 14:14:03	U SMPL
K3421-02 - 1	SAMPLE-1	697	0.1469	-	7471B	PPB	18 Jun 2019 14:16:20	U SMPL
K3421-06 - 1	SAMPLE-2	232	0.0634	-	7471B	PPB	18 Jun 2019 14:18:36	U SMPL
PB120716BL - 1	PBS	-136	-0.0028	-	7471B	PPB	18 Jun 2019 14:20:51	U SMPL
PB120716BS - 1	LCSS	20165	3.6457	-	7471B	PPB	18 Jun 2019 14:23:08	U SMPL
K3154-01 - 1	JC-02-061419-A	11542	2.0960	-	7471B	PPB	18 Jun 2019 14:25:25	U SMPL
K3154-01DUP - 1	JC-02-061419-ADUP	11436	2.0770	-	7471B	PPB	18 Jun 2019 14:27:42	U SMPL
K3154-01MS - 1	JC-02-061419-AMS	31931	5.7603	-	7471B	PPB	18 Jun 2019 14:29:59	U SMPL
K3154-01MSD - 1	JC-02-061419-AMSD	32542	5.8701	-	7471B	PPB	18 Jun 2019 14:32:16	U SMPL
K3154-03 - 1	JC-02-061419-B	14592	2.6441	-	7471B	PPB	18 Jun 2019 14:34:33	U SMPL
CCV88 - 1	CCV88	27885	5.0331	-	7471B	PPB	18 Jun 2019 14:36:49	U SMPL
CCB88 - 1	CCB88	-206	-0.0153	-	7471B	PPB	18 Jun 2019 14:39:05	U SMPL
K3154-05 - 1	JC-02-061419-C	6319	1.1573	-	7471B	PPB	18 Jun 2019 14:41:21	U SMPL
K3154-07 - 1	JC-02-061419-D	9072	1.6521	-	7471B	PPB	18 Jun 2019 14:43:37	U SMPL
K3154-09 - 1	JC-02-061419-E	10562	1.9199	-	7471B	PPB	18 Jun 2019 14:45:53	U SMPL
K3154-11 - 1	JC-02-061419-F	13591	2.4642	-	7471B	PPB	18 Jun 2019 14:48:09	U SMPL
K3154-13 - 1	JC-02-061419-G	20209	3.6536	-	7471B	PPB	18 Jun 2019 14:50:26	U SMPL
K3163-09 - 1	SU-03-061719-A	1211	0.2393	-	7471B	PPB	18 Jun 2019 14:52:42	U SMPL
K3163-11 - 1	SU-03-061719-B	824	0.1698	-	7471B	PPB	18 Jun 2019 14:54:59	U SMPL
K3366-04 - 1	BRANCH-LEAVES	277	0.0715	-	7471B	PPB	18 Jun 2019 14:57:16	U SMPL
K3376-01 - 1	NEW-DOVER-TP	782	0.1622	-	7471B	PPB	18 Jun 2019 14:59:33	U SMPL
K3382-05 - 1	GRAVEL-1	-89	0.0057	-	7471B	PPB	18 Jun 2019 15:01:49	U SMPL
CCV89 - 1	CCV89	27265	4.9217	-	7471B	PPB	18 Jun 2019 15:04:05	U SMPL
CCB89 - 1	CCB89	-179	-0.0105	-	7471B	PPB	18 Jun 2019 15:06:21	U SMPL
K3382-07 - 1	GRAVEL-2	-86	0.0062	-	7471B	PPB	18 Jun 2019 15:08:38	U SMPL
K3389-01 - 1	GS-SOIL-PILE	2742	0.5145	-	7471B	PPB	18 Jun 2019 15:10:54	U SMPL
K3406-02 - 1	BAT-B14	2745	0.5150	-	7471B	PPB	18 Jun 2019 15:13:10	U SMPL
K3409-01 - 1	T-1	53643	9.6623	-	7471B	PPB	18 Jun 2019 15:15:25	U SMPL
K3420-02LX5 - 1		8	0.0231	-	7471B	PPB	18 Jun 2019 15:26:27	U SMPL
K3420-02A - 1		20694	3.7408	-	7471B	PPB	18 Jun 2019 15:28:44	U SMPL
K3154-01LX5 - 1		2009	0.3827	-	7471B	PPB	18 Jun 2019 15:31:00	U SMPL
K3154-01A - 1		31333	5.6528	-	7471B	PPB	18 Jun 2019 15:33:18	U SMPL
CCV90 - 1	CCV90	27523	4.9681	-	7471B	PPB	18 Jun 2019 15:35:35	U SMPL
CCB90 - 1	CCB90	-202	-0.0146	-	7471B	PPB	18 Jun 2019 15:37:52	U SMPL