

2B163504

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/19/2019 12:57

Test: *Reactive*
~~Total~~ CN *Mg/L*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.039	0.0	0.098	
ICB1	0.677	0.0	0.003	
CCV1	241.718	0.0	0.243	
CCB1	0.634	0.0	0.003	
PB120762BL	0.587	0.0	0.003	
K3441-04	0.505	0.0	0.003	
K3441-04DUP	0.376	0.0	0.003	
PB120763BL	0.463	0.0	0.003	
K3433-02	-0.214	0.0	0.003	
K3433-02DUP	0.496	0.0	0.003	
K3441-06	0.688	0.0	0.003	
CCV2	255.156	0.0	0.256	
CCB2	0.731	0.0	0.003	

N	13
Mean	45.989
SD	93.6590
CV%	203.66

Aquakem v. 7.2AQ1

Results from time period:

Wed Jun 19 09:45:10 2019

Wed Jun 19 12:43:56 2019

✓ AS

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	0.4309	µg/l	6/19/2019 9:45:10	
5.0PPBCN	A	Reactive CN	P	5.4643	µg/l	6/19/2019 9:45:11	
10PPBCN	A	Reactive CN	P	10.4408	µg/l	6/19/2019 9:45:12	
50PPBCN	A	Reactive CN	P	50.1427	µg/l	6/19/2019 9:45:13	
100PPBCN	A	Reactive CN	P	98.1555	µg/l	6/19/2019 9:45:14	
250PPBCN	A	Reactive CN	P	250.0491	µg/l	6/19/2019 9:45:15	
500PPBCN	A	Reactive CN	P	500.3167	µg/l	6/19/2019 9:45:16	
ICV1	S	Reactive CN	P	96.0386	µg/l	6/19/2019 12:40:32	
ICB1	S	Reactive CN	P	0.6765	µg/l	6/19/2019 12:40:33	
CCV1	S	Reactive CN	P	241.7181	µg/l	6/19/2019 12:40:34	
CCB1	S	Reactive CN	P	0.6337	µg/l	6/19/2019 12:40:35	
PB120762BL	S	Reactive CN	P	0.587	µg/l	6/19/2019 12:40:36	
K3441-04	S	Reactive CN	P	0.5051	µg/l	6/19/2019 12:40:37	
K3441-04DUP	S	Reactive CN	P	0.3764	µg/l	6/19/2019 12:40:38	
PB120763BL	S	Reactive CN	P	0.4628	µg/l	6/19/2019 12:40:39	
K3433-02	S	Reactive CN	P	-0.214	µg/l	6/19/2019 12:40:40	
K3433-02DUP	S	Reactive CN	P	0.4957	µg/l	6/19/2019 12:40:41	
K3441-06	S	Reactive CN	P	0.6876	µg/l	6/19/2019 12:40:42	
CCV2	S	Reactive CN	P	255.156	µg/l	6/19/2019 12:43:55	
CCB2	S	Reactive CN	P	0.7306	µg/l	6/19/2019 12:43:56	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/19/2019 9:48


Test Total CN

Accepted 6/19/2019 9:48

Factor 1006
Bias 0.003

Coeff. of det. 0.999980

Errors

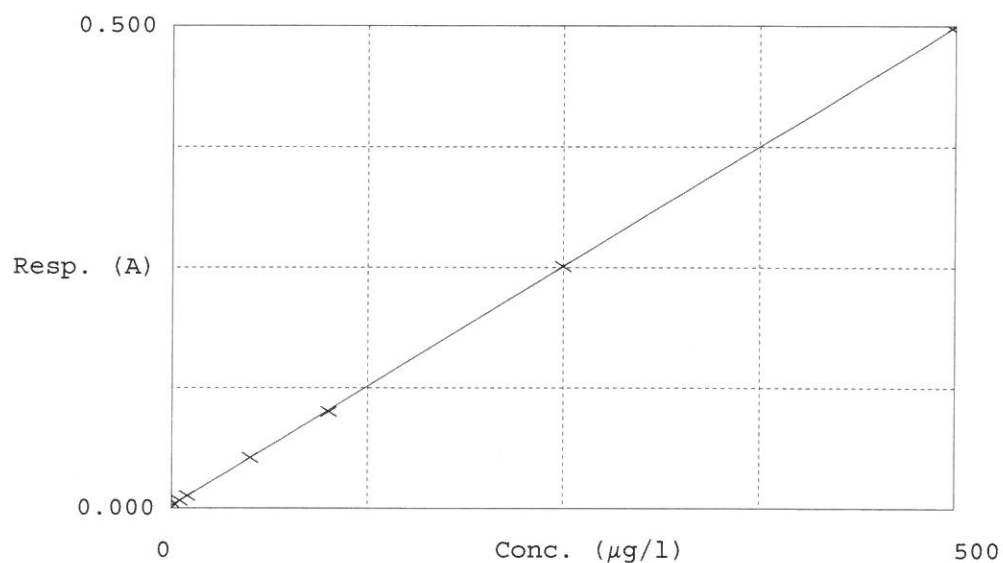

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	0.4309	0.0000	
2	5.0PPBCN	0.008	5.4643	5.0000	
3	10PPBCN	0.013	10.4408	10.0000	
4	50PPBCN	0.053	50.1427	50.0000	
5	100PPBCN	0.100	98.1555	100.0000	
6	250PPBCN	0.251	250.0491	250.0000	
7	500PPBCN	0.500	500.3167	500.0000	