

=====

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/19/2019 15:22

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.814	0.0	0.096	
ICB1	0.806	0.0	0.004	
CCV1	238.778	0.0	0.240	
CCB1	0.796	0.0	0.004	
PB120761BL	0.694	0.0	0.003	
PB120761BS	95.445	0.0	0.098	
LOWPB120761	10.313	0.0	0.013	
HIGHPB120761	496.367	0.0	0.496	
K3435-01	1.229	0.0	0.004	
K3435-01DUP	0.898	0.0	0.004	
K3435-01MS	37.032	0.0	0.040	
K3435-01MSD	36.710	0.0	0.039	
K3435-03	0.596	0.0	0.003	
K3438-01	1.286	0.0	0.004	
CCV2	241.663	0.0	0.243	
CCB2	0.824	0.0	0.004	
K3438-03	1.013	0.0	0.004	
K3439-01	5.141	0.0	0.008	
K3440-01	0.605	0.0	0.003	
K3440-03	0.707	0.0	0.003	
K3441-02	0.946	0.0	0.004	
CCV3	240.148	0.0	0.241	
CCB3	0.359	0.0	0.003	

N	23
Mean	65.486
SD	124.6097
CV%	190.29

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

6/19/2019 9:48


Test Total CN

Accepted 6/19/2019 9:48

Factor 1006
Bias 0.003

Coeff. of det. 0.999980

Errors

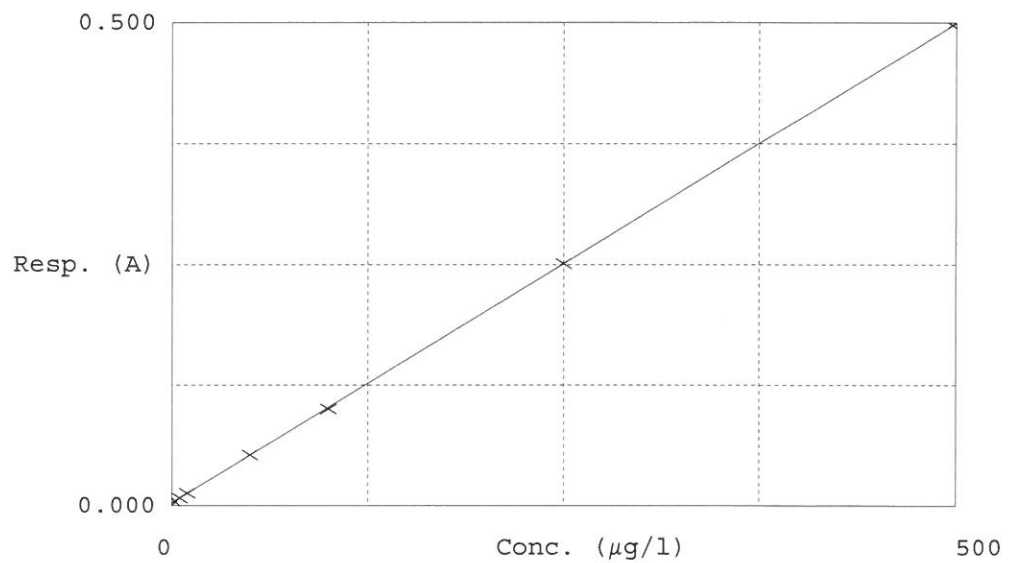

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	0.4309	0.0000	
2	5.0PPBCN	0.008	5.4643	5.0000	
3	10PPBCN	0.013	10.4408	10.0000	
4	50PPBCN	0.053	50.1427	50.0000	
5	100PPBCN	0.100	98.1555	100.0000	
6	250PPBCN	0.251	250.0491	250.0000	
7	500PPBCN	0.500	500.3167	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Wed Jun 19 15:04:37 2019

Wed Jun 19 15:15:57 2019

AS

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive	Cl P	0.4309	µg/l	6/19/2019 9:45:10	
5.OPPBCN	A	Reactive	Cl P	5.4643	µg/l	6/19/2019 9:45:11	
10PPBCN	A	Reactive	Cl P	10.4408	µg/l	6/19/2019 9:45:12	
50PPBCN	A	Reactive	Cl P	50.1427	µg/l	6/19/2019 9:45:13	
100PPBCN	A	Reactive	Cl P	98.1555	µg/l	6/19/2019 9:45:14	
250PPBCN	A	Reactive	Cl P	250.0491	µg/l	6/19/2019 9:45:15	
500PPBCN	A	Reactive	Cl P	500.3167	µg/l	6/19/2019 9:45:16	
ICV1	S	Total	CN P	93.8144	µg/l	6/19/2019 15:04:37	
ICB1	S	Total	CN P	0.8059	µg/l	6/19/2019 15:04:38	
CCV1	S	Total	CN P	238.7778	µg/l	6/19/2019 15:04:39	
CCB1	S	Total	CN P	0.796	µg/l	6/19/2019 15:04:40	
PB120761BL	S	Total	CN P	0.6938	µg/l	6/19/2019 15:04:41	
PB120761BS	S	Total	CN P	95.4453	µg/l	6/19/2019 15:04:42	
LOWPB120761	S	Total	CN P	10.3127	µg/l	6/19/2019 15:04:43	
HIGHPB120761	S	Total	CN P	496.3665	µg/l	6/19/2019 15:04:44	
K3435-01	S	Total	CN P	1.2288	µg/l	6/19/2019 15:04:45	
K3435-01DUP	S	Total	CN P	0.8983	µg/l	6/19/2019 15:04:46	
K3435-01MS	S	Total	CN P	37.0319	µg/l	6/19/2019 15:04:47	
K3435-01MSD	S	Total	CN P	36.7098	µg/l	6/19/2019 15:12:12	
K3435-03	S	Total	CN P	0.5964	µg/l	6/19/2019 15:12:13	
K3438-01	S	Total	CN P	1.2857	µg/l	6/19/2019 15:12:14	
CCV2	S	Total	CN P	241.6634	µg/l	6/19/2019 15:12:15	
CCB2	S	Total	CN P	0.8238	µg/l	6/19/2019 15:12:16	
K3438-03	S	Total	CN P	1.0132	µg/l	6/19/2019 15:12:17	
K3439-01	S	Total	CN P	5.1411	µg/l	6/19/2019 15:12:18	
K3440-01	S	Total	CN P	0.6049	µg/l	6/19/2019 15:12:19	
K3440-03	S	Total	CN P	0.7073	µg/l	6/19/2019 15:12:20	
K3441-02	S	Total	CN P	0.9457	µg/l	6/19/2019 15:12:21	
CCV3	S	Total	CN P	240.148	µg/l	6/19/2019 15:12:22	
CCB3	S	Total	CN P	0.3587	µg/l	6/19/2019 15:15:56	