


LB103565

245.1

INSTRUMENT ID : CU1

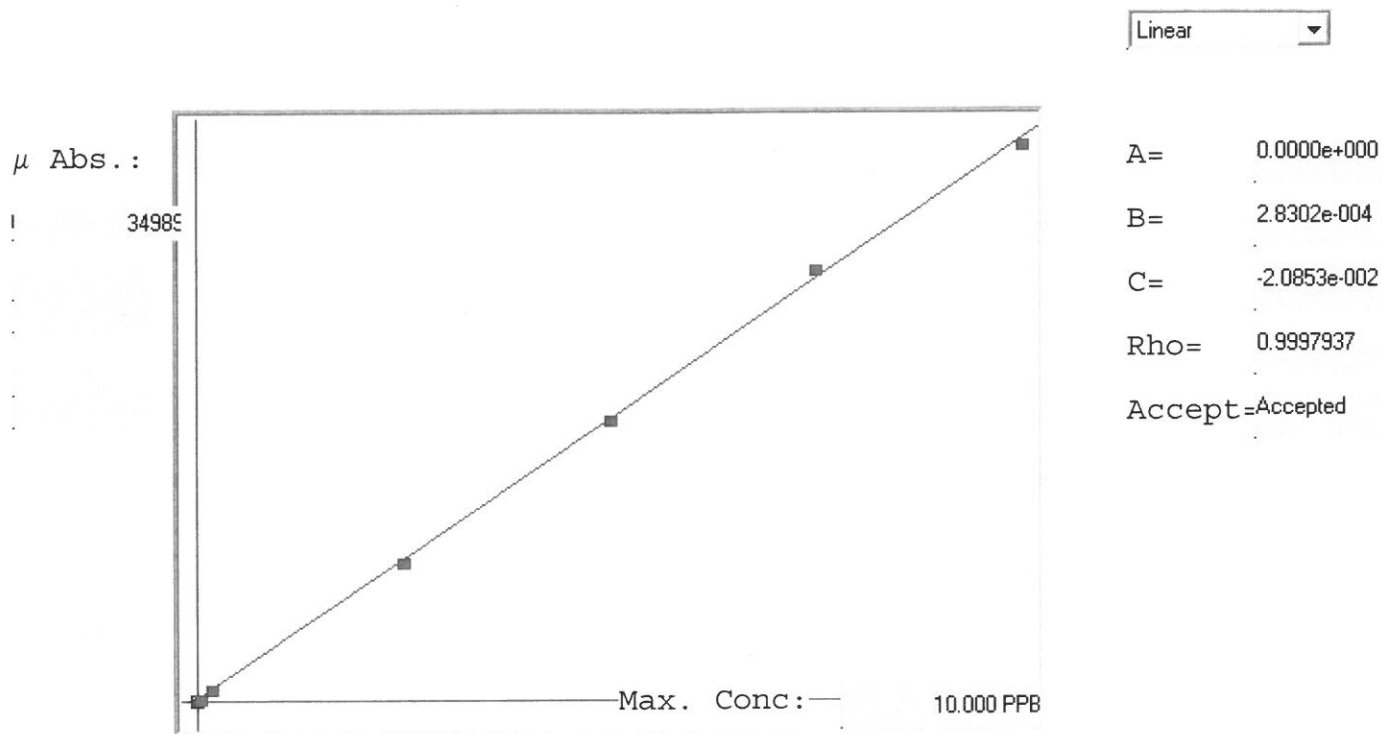

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.008	-0.008	45	0.000	45				
0.05	0.050	0.047	-0.003	239	0.0 %	239				
0.2	0.200	0.195	-0.005	762	0.0 %	762				
2.5	2.500	2.469	-0.031	8799	0.0 %	8799				
5.0	5.000	5.008	0.008	17768	0.0 %	17768				
7.5	7.500	7.657	0.157	27129	0.0 %	27129				
10.0	10.000	9.882	-0.118	34989	0.0 %	34989				

LB103565 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 21 Jun 2019 16:15:29

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	45	-	0.0000	245.1	PPB	21 Jun 2019 16:58:24	S	Std
0.05 - 1	50.05	239	-	0.0500	245.1	PPB	21 Jun 2019 17:00:41	S	Std
0.2 - 1	50.2	762	-	0.2000	245.1	PPB	21 Jun 2019 17:02:59	S	Std
2.5 - 1	52.5	8799	-	2.5000	245.1	PPB	21 Jun 2019 17:05:16	S	Std
5.0 - 1	55.0	17768	-	5.0000	245.1	PPB	21 Jun 2019 17:07:33	S	Std
7.5 - 1	57.5	27129	-	7.5000	245.1	PPB	21 Jun 2019 17:09:49	S	Std
10.0 - 1	510.0	34989	-	10.0000	245.1	PPB	21 Jun 2019 17:17:39	S	Std
ICV07 - 1	ICV07	14610	4.1141	-245.1		PPB	21 Jun 2019 17:20:18	U	SMPL
ICB07 - 1	ICB07	-99	-0.0489	-245.1		PPB	21 Jun 2019 17:22:34	U	SMPL
CCV17 - 1	CCV17	17482	4.9270	-245.1		PPB	21 Jun 2019 17:24:49	U	SMPL
CCB17 - 1	CCB17	-61	-0.0381	-245.1		PPB	21 Jun 2019 17:27:05	U	SMPL
CRA - 1	CRA	199	0.0355	-245.1		PPB	21 Jun 2019 17:29:20	U	SMPL
HighStd - 1	HighStd	34799	9.8281	-245.1		PPB	21 Jun 2019 17:31:36	U	SMPL
ChkStd - 1	ChkStd	24257	6.8444	-245.1		PPB	21 Jun 2019 17:33:52	U	SMPL
PB120828BL - 1	PBW	-176	-0.0707	-245.1		PPB	21 Jun 2019 17:36:11	U	SMPL
PB120828BS - 1	LCSW	15111	4.2559	-245.1		PPB	21 Jun 2019 17:38:33	U	SMPL
K3299-04 - 1	TI-658	136	0.0176	-245.1		PPB	21 Jun 2019 17:40:53	U	SMPL
K3299-04DUP - 1	TI-658DUP	175	0.0287	-245.1		PPB	21 Jun 2019 17:43:28	U	SMPL
K3299-04MS - 1	TI-658MS	14974	4.2171	-245.1		PPB	21 Jun 2019 17:45:47	U	SMPL
K3299-04MSD - 1	TI-658MSD	15094	4.2511	-245.1		PPB	21 Jun 2019 17:48:05	U	SMPL
K3300-06 - 1	TI-633	-96	-0.0480	-245.1		PPB	21 Jun 2019 17:50:21	U	SMPL
CCV18 - 1	CCV18	17909	5.0478	-245.1		PPB	21 Jun 2019 17:52:37	U	SMPL
CCB18 - 1	CCB18	-161	-0.0664	-245.1		PPB	21 Jun 2019 17:54:53	U	SMPL
K3299-04LX5 - 1		-120	-0.0548	-245.1		PPB	21 Jun 2019 17:57:09	U	SMPL
K3299-04A - 1		14944	4.2086	-245.1		PPB	21 Jun 2019 17:59:24	U	SMPL
CCV19 - 1	CCV19	17928	5.0532	-245.1		PPB	21 Jun 2019 18:01:41	U	SMPL
CCB19 - 1	CCB19	-68	-0.0401	-245.1		PPB	21 Jun 2019 18:03:57	U	SMPL