


LB103606

7470A

INSTRUMENT ID : CU1

Linear

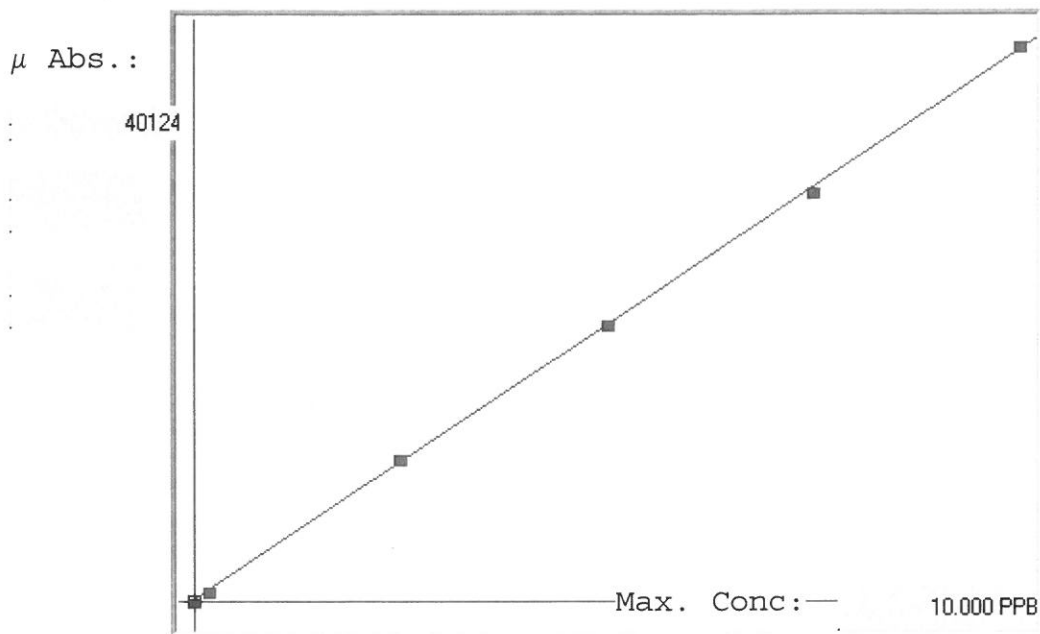

A= 0.0000e+000

B= 2.5139e-004

C= -3.4310e-002

Rho= 0.9998940

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.002	-0.002	127	0.000	127				
0.2	0.200	0.174	-0.026	830	0.0 %	830				
2.5	2.500	2.574	0.074	10374	0.0 %	10374				
5.0	5.000	4.994	-0.006	20003	0.0 %	20003				
7.5	7.500	7.408	-0.092	29605	0.0 %	29605				
10.0	10.000	10.052	0.052	40124	0.0 %	40124				

LB103606 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 25 Jun 2019 13:09:12

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	127	-	0.0000	7470A	PPB	25 Jun 2019 13:09:27	S	Std
0.2 - 1	50.2	830	-	0.2000	7470A	PPB	25 Jun 2019 13:11:35	S	Std
2.5 - 1	52.5	10374	-	2.5000	7470A	PPB	25 Jun 2019 13:13:44	S	Std
5.0 - 1	55.0	20003	-	5.0000	7470A	PPB	25 Jun 2019 13:15:52	S	Std
7.5 - 1	57.5	29605	-	7.5000	7470A	PPB	25 Jun 2019 13:18:00	S	Std
10.0 - 1	510.0	40124	-	10.0000	7470A	PPB	25 Jun 2019 13:20:07	S	Std
ICV09 - 1	ICV09	15828	3.9446	-	7470A	PPB	25 Jun 2019 13:23:17	U	SMPL
ICB09 - 1	ICB09	29	-0.0270	-	7470A	PPB	25 Jun 2019 13:25:23	U	SMPL
CCV27 - 1	CCV27	19599	4.8926	-	7470A	PPB	25 Jun 2019 13:27:30	U	SMPL
CCB27 - 1	CCB27	34	-0.0258	-	7470A	PPB	25 Jun 2019 13:29:36	U	SMPL
CRA - 1	CRA	822	0.1723	-	7470A	PPB	25 Jun 2019 13:31:43	U	SMPL
HighStd - 1	HighStd	39962	10.0116	-	7470A	PPB	25 Jun 2019 13:33:49	U	SMPL
ChkStd - 1	ChkStd	27630	6.9115	-	7470A	PPB	25 Jun 2019 13:35:56	U	SMPL
PB120897BL - 1	PBW	116	-0.0051	-	7470A	PPB	25 Jun 2019 13:38:04	U	SMPL
PB120897BS - 1	LCSW	13513	3.3627	-	7470A	PPB	25 Jun 2019 13:40:11	U	SMPL
K3482-02 - 1	TP-1	79	-0.0144	-	7470A	PPB	25 Jun 2019 13:42:19	U	SMPL
K3482-02DUP - 1	TP-1DUP	112	-0.0062	-	7470A	PPB	25 Jun 2019 13:44:27	U	SMPL
K3482-02MS - 1	TP-1MS	15488	3.8592	-	7470A	PPB	25 Jun 2019 13:52:46	U	SMPL
K3482-02MSD - 1	TP-1MSD	15682	3.9079	-	7470A	PPB	25 Jun 2019 13:54:55	U	SMPL
K3482-04 - 1	TP-2	96	-0.0102	-	7470A	PPB	25 Jun 2019 13:57:04	U	SMPL
CCV28 - 1	CCV28	20082	5.0140	-	7470A	PPB	25 Jun 2019 13:59:12	U	SMPL
CCB28 - 1	CCB28	63	-0.0185	-	7470A	PPB	25 Jun 2019 14:01:22	U	SMPL
K3482-06 - 1	TP-3	81	-0.0139	-	7470A	PPB	25 Jun 2019 14:03:33	U	SMPL
K3482-08 - 1	TP-4	122	-0.0036	-	7470A	PPB	25 Jun 2019 14:05:41	U	SMPL
PB120898BL - 1	PBW	162	0.0064	-	7470A	PPB	25 Jun 2019 14:07:48	U	SMPL
PB120898BS - 1	LCSW	13697	3.4089	-	7470A	PPB	25 Jun 2019 14:09:55	U	SMPL
K3485-02 - 1	GWMH-7	89	-0.0119	-	7470A	PPB	25 Jun 2019 14:12:02	U	SMPL
K3485-02DUP - 1	GWMH-7DUP	-5	-0.0356	-	7470A	PPB	25 Jun 2019 14:14:09	U	SMPL
K3485-02MS - 1	GWMH-7MS	15709	3.9147	-	7470A	PPB	25 Jun 2019 14:21:12	U	SMPL
K3485-02MSD - 1	GWMH-7MSD	15578	3.8818	-	7470A	PPB	25 Jun 2019 14:23:19	U	SMPL
PB120899BL - 1	PBW	147	0.0026	-	7470A	PPB	25 Jun 2019 14:25:27	U	SMPL
PB120899BS - 1	LCSW	13476	3.3534	-	7470A	PPB	25 Jun 2019 14:27:34	U	SMPL
CCV29 - 1	CCV29	19582	4.8883	-	7470A	PPB	25 Jun 2019 14:29:41	U	SMPL
CCB29 - 1	CCB29	50	-0.0217	-	7470A	PPB	25 Jun 2019 14:31:47	U	SMPL
K3485-01 - 1	GWMH-7	1839	0.4280	-	7470A	PPB	25 Jun 2019 14:33:54	U	SMPL
K3486-01 - 1	W-1	-19	-0.0391	-	7470A	PPB	25 Jun 2019 14:36:01	U	SMPL
K3486-02 - 1	W-2	24	-0.0283	-	7470A	PPB	25 Jun 2019 14:38:08	U	SMPL
K3486-03 - 1	W-3	-105	-0.0607	-	7470A	PPB	25 Jun 2019 14:40:14	U	SMPL
K3486-04 - 1	W-4	127	-0.0024	-	7470A	PPB	25 Jun 2019 14:42:22	U	SMPL
K3486-04DUP - 1	W-4DUP	116	-0.0051	-	7470A	PPB	25 Jun 2019 14:44:29	U	SMPL
K3486-04MS - 1	W-4MS	15218	3.7913	-	7470A	PPB	25 Jun 2019 14:49:09	U	SMPL
K3486-04MSD - 1	W-4MSD	15099	3.7614	-	7470A	PPB	25 Jun 2019 14:51:16	U	SMPL
K3499-09 - 1	TWP-B-6	-116	-0.0635	-	7470A	PPB	25 Jun 2019 14:53:24	U	SMPL
K3500-09 - 1	GW-A-061919	-65	-0.0506	-	7470A	PPB	25 Jun 2019 14:55:31	U	SMPL
CCV30 - 1	CCV30	20170	5.0362	-	7470A	PPB	25 Jun 2019 14:57:38	U	SMPL
CCB30 - 1	CCB30	-236	-0.0936	-	7470A	PPB	25 Jun 2019 14:59:48	U	SMPL
K3500-10 - 1	GW-B-061919	-53	-0.0476	-	7470A	PPB	25 Jun 2019 15:01:57	U	SMPL
K3511-05 - 1	N43502	-19	-0.0391	-	7470A	PPB	25 Jun 2019 15:04:04	U	SMPL
PB120897TB - 1	PB120833TB	97	-0.0099	-	7470A	PPB	25 Jun 2019 15:06:11	U	SMPL
PB120898TB - 1	PB120840TB	85	-0.0129	-	7470A	PPB	25 Jun 2019 15:08:18	U	SMPL
K3482-02LX5 - 1		3	-0.0336	-	7470A	PPB	25 Jun 2019 15:10:25	U	SMPL
K3482-02A - 1		15112	3.7646	-	7470A	PPB	25 Jun 2019 15:12:33	U	SMPL
K3485-02LX5 - 1		-21	-0.0396	-	7470A	PPB	25 Jun 2019 15:14:40	U	SMPL
K3485-02A - 1		16564	4.1297	-	7470A	PPB	25 Jun 2019 15:24:02	U	SMPL
K3486-04LX5 - 1		-24	-0.0403	-	7470A	PPB	25 Jun 2019 15:26:10	U	SMPL
K3486-04A - 1		16631	4.1465	-	7470A	PPB	25 Jun 2019 15:28:17	U	SMPL
CCV31 - 1	CCV31	19598	4.8924	-	7470A	PPB	25 Jun 2019 15:30:24	U	SMPL
CCB31 - 1	CCB31	41	-0.0240	-	7470A	PPB	25 Jun 2019 15:32:31	U	SMPL