


LB103685

7471B

INSTRUMENT ID: CV1

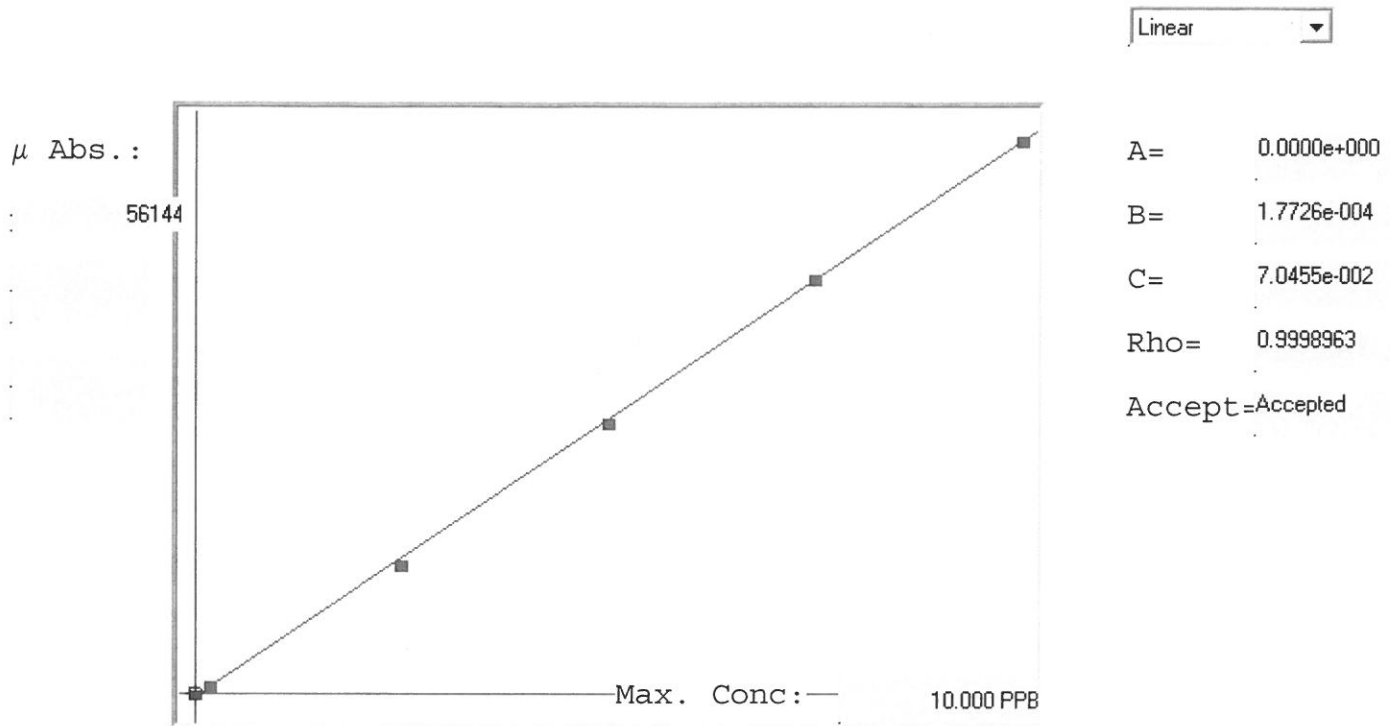

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.054	0.054	-95	0.000	-95				
0.2	0.200	0.235	0.035	926	0.0 %	926				
2.5	2.500	2.414	-0.086	13220	0.0 %	13220				
5.0	5.000	4.940	-0.060	27470	0.0 %	27470				
7.5	7.500	7.536	0.036	42118	0.0 %	42118				
10.0	10.000	10.022	0.022	56144	0.0 %	56144				

LB103685 INSTRUMENT ID : CV1

Method: 7471B	Operator: Admin	Date of Analysis: 28 Jun 2019 09:44:38							
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	-95	-	0.00007471B	PPB		28 Jun 2019 09:48:10	S	Std
0.2 - 1	50.2	926	-	0.20007471B	PPB		28 Jun 2019 09:50:30	S	Std
2.5 - 1	52.5	13220	-	2.50007471B	PPB		28 Jun 2019 09:52:48	S	Std
5.0 - 1	55.0	27470	-	5.00007471B	PPB		28 Jun 2019 09:55:05	S	Std
7.5 - 1	57.5	42118	-	7.50007471B	PPB		28 Jun 2019 09:57:22	S	Std
10.0 - 1	510.0	56144	-	10.00007471B	PPB		28 Jun 2019 09:59:39	S	Std
ICV15 - 1	ICV15	22202	4.0059	-7471B	PPB		28 Jun 2019 10:02:42	U	SMPL
ICB15 - 1	ICB15	-125	0.0483	-7471B	PPB		28 Jun 2019 10:04:58	U	SMPL
CCV58 - 1	CCV58	27562	4.9560	-7471B	PPB		28 Jun 2019 10:07:14	U	SMPL
CCB58 - 1	CCB58	-130	0.0474	-7471B	PPB		28 Jun 2019 10:09:29	U	SMPL
CRA - 1	CRA	888	0.2279	-7471B	PPB		28 Jun 2019 10:11:45	U	SMPL
HighStd - 1	HighStd	56331	10.0554	-7471B	PPB		28 Jun 2019 10:14:00	U	SMPL
ChkStd - 1	ChkStd	39564	7.0834	-7471B	PPB		28 Jun 2019 10:16:17	U	SMPL
PB121013BL - 1	PBS	-94	0.0538	-7471B	PPB		28 Jun 2019 10:18:34	U	SMPL
PB121013BS - 1	LCSS	19407	3.5104	-7471B	PPB		28 Jun 2019 10:20:54	U	SMPL
K3158-07 - 1	OK-02-062719	1144	0.2732	-7471B	PPB		28 Jun 2019 10:23:14	U	SMPL
K3158-07DUP - 1	OK-02-062719DUP	1140	0.2725	-7471B	PPB		28 Jun 2019 10:25:33	U	SMPL
K3158-07MS - 1	OK-02-062719MS	21778	3.9307	-7471B	PPB		28 Jun 2019 10:27:51	U	SMPL
K3158-07MSD - 1	OK-02-062719MSD	22583	4.0734	-7471B	PPB		28 Jun 2019 10:30:08	U	SMPL
K3163-13 - 1	SU-01-062719-A	1665	0.3656	-7471B	PPB		28 Jun 2019 10:32:24	U	SMPL
CCV59 - 1	CCV59	27827	5.0029	-7471B	PPB		28 Jun 2019 10:34:40	U	SMPL
CCB59 - 1	CCB59	-109	0.0511	-7471B	PPB		28 Jun 2019 10:36:55	U	SMPL
K3163-15 - 1	SU-01-062719-B	1046	0.2559	-7471B	PPB		28 Jun 2019 10:39:12	U	SMPL
K3554-02 - 1	SAMPLE-11	1668	0.3661	-7471B	PPB		28 Jun 2019 10:41:28	U	SMPL
K3554-06 - 1	SAMPLE-15	551	0.1681	-7471B	PPB		28 Jun 2019 10:43:44	U	SMPL
K3554-10 - 1	SAMPLE-16	520	0.1626	-7471B	PPB		28 Jun 2019 10:46:00	U	SMPL
K3555-02 - 1	SAMPLE-17	634	0.1828	-7471B	PPB		28 Jun 2019 10:48:16	U	SMPL
K3555-06 - 1	SAMPLE-18	144	0.0960	-7471B	PPB		28 Jun 2019 10:50:33	U	SMPL
K3555-10 - 1	SAMPLE-9	1312	0.3030	-7471B	PPB		28 Jun 2019 10:52:50	U	SMPL
K3555-14 - 1	SAMPLE-12	1125	0.2699	-7471B	PPB		28 Jun 2019 10:55:07	U	SMPL
K3555-18 - 1	SAMPLE-13	519	0.1625	-7471B	PPB		28 Jun 2019 10:57:25	U	SMPL
K3555-22 - 1	SAMPLE-14	333	0.1295	-7471B	PPB		28 Jun 2019 10:59:41	U	SMPL
CCV60 - 1	CCV60	28062	5.0446	-7471B	PPB		28 Jun 2019 11:01:57	U	SMPL
CCB60 - 1	CCB60	-151	0.0437	-7471B	PPB		28 Jun 2019 11:04:13	U	SMPL
K3563-01 - 1	SOIL-COMP-1	1164	0.2768	-7471B	PPB		28 Jun 2019 11:06:31	U	SMPL
K3563-03 - 1	SOIL-COMP-2	641	0.1841	-7471B	PPB		28 Jun 2019 11:08:48	U	SMPL
K3573-01 - 1	SR-SOIL-COMP-1	483	0.1561	-7471B	PPB		28 Jun 2019 11:11:04	U	SMPL
K3573-02 - 1	SR-SOIL-COMP-2	405	0.1422	-7471B	PPB		28 Jun 2019 11:13:20	U	SMPL
K3576-01 - 1	SP-1	39179	7.0151	-7471B	PPB		28 Jun 2019 11:15:37	U	SMPL
K3582-01 - 1	FK-PS-01-049	1785	0.3869	-7471B	PPB		28 Jun 2019 11:17:53	U	SMPL
K3584-01 - 1	FK-0D015-03-009	1582	0.3509	-7471B	PPB		28 Jun 2019 11:20:12	U	SMPL
K3158-07LX5 - 1		102	0.0885	-7471B	PPB		28 Jun 2019 11:22:29	U	SMPL
K3158-07A - 1		22635	4.0826	-7471B	PPB		28 Jun 2019 11:24:46	U	SMPL
CCV61 - 1	CCV61	28504	5.1229	-7471B	PPB		28 Jun 2019 11:27:03	U	SMPL
CCB61 - 1	CCB61	-144	0.0449	-7471B	PPB		28 Jun 2019 11:29:19	U	SMPL