


LB103755

7471B

INSTRUMENT ID : CU1

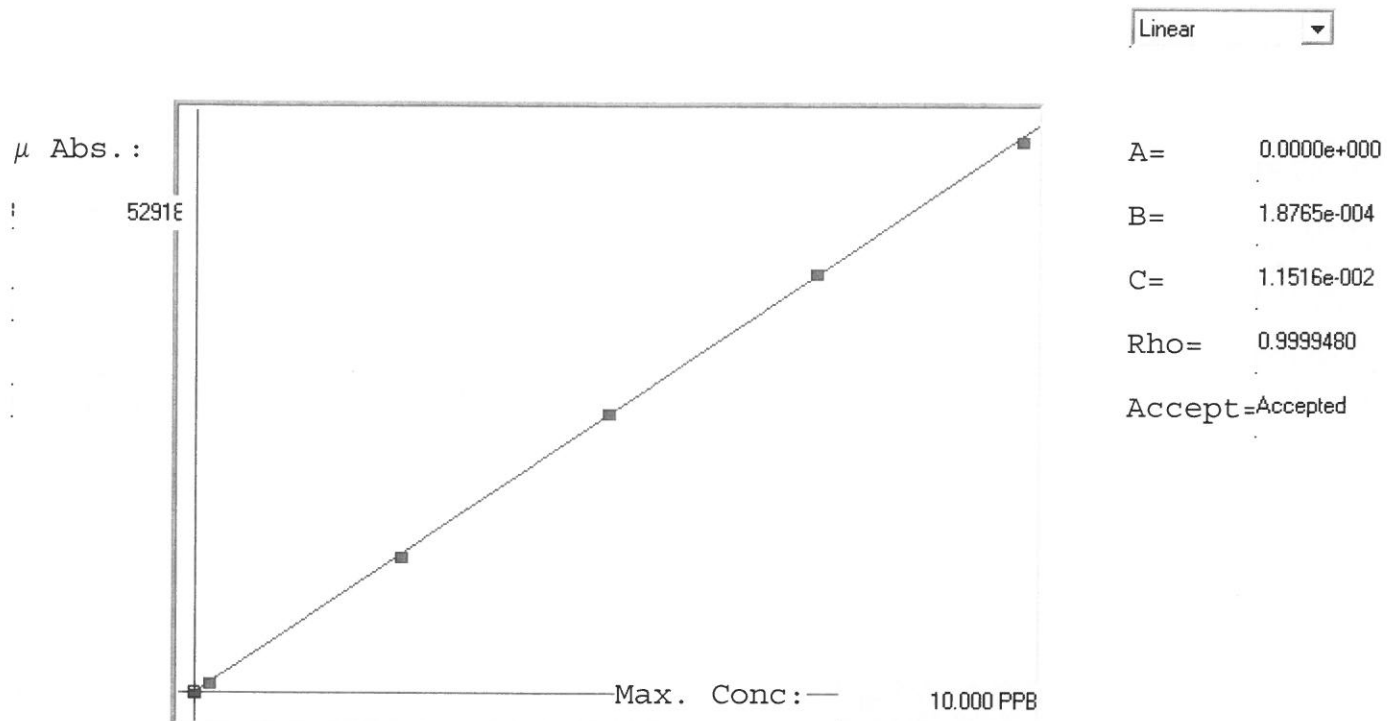

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.009	-0.009	-110	0.000	-110				
0.2	0.200	0.185	-0.015	922	0.0 %	922				
2.5	2.500	2.488	-0.012	13195	0.0 %	13195				
5.0	5.000	5.042	0.042	26810	0.0 %	26810				
7.5	7.500	7.553	0.053	40189	0.0 %	40189				
10.0	10.000	9.942	-0.058	52918	0.0 %	52918				

LB103755 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 02 Jul 2019 09:00:54

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	-110	-	0.0000	7471B	PPB	02 Jul 2019 09:22:35	S	Std
0.2 - 1	50.2	922	-	0.2000	7471B	PPB	02 Jul 2019 09:24:58	S	Std
2.5 - 1	52.5	13195	-	2.5000	7471B	PPB	02 Jul 2019 09:27:16	S	Std
5.0 - 1	55.0	26810	-	5.0000	7471B	PPB	02 Jul 2019 09:29:34	S	Std
7.5 - 1	57.5	40189	-	7.5000	7471B	PPB	02 Jul 2019 09:31:51	S	Std
10.0 - 1	510.0	52918	-	10.0000	7471B	PPB	02 Jul 2019 09:34:08	S	Std
ICV17 - 1	ICV17	22390	4.2130	-7471B	PPB	PPB	02 Jul 2019 09:38:09	U	SMPL
ICB17 - 1	ICB17	-130	-0.0129	-7471B	PPB	PPB	02 Jul 2019 09:40:25	U	SMPL
CCV69 - 1	CCV69	27027	5.0831	-7471B	PPB	PPB	02 Jul 2019 09:42:42	U	SMPL
CCB69 - 1	CCB69	-143	-0.0153	-7471B	PPB	PPB	02 Jul 2019 09:44:57	U	SMPL
CRA - 1	CRA	934	0.1868	-7471B	PPB	PPB	02 Jul 2019 09:47:14	U	SMPL
HighStd - 1	HighStd	52896	9.9375	-7471B	PPB	PPB	02 Jul 2019 09:49:30	U	SMPL
ChkStd - 1	ChkStd	37126	6.9782	-7471B	PPB	PPB	02 Jul 2019 09:51:45	U	SMPL
PB121098BL - 1	PBS	-151	-0.0168	-7471B	PPB	PPB	02 Jul 2019 09:54:04	U	SMPL
PB121098BS - 1	LCSS	19948	3.7548	-7471B	PPB	PPB	02 Jul 2019 09:56:22	U	SMPL
K3158-09 - 1	OK-01-062819	3669	0.7000	-7471B	PPB	PPB	02 Jul 2019 09:58:38	U	SMPL
K3158-09DUP - 1	OK-01-062819DUP	3551	0.6779	-7471B	PPB	PPB	02 Jul 2019 10:00:55	U	SMPL
K3158-09MS - 1	OK-01-062819MS	28474	5.3547	-7471B	PPB	PPB	02 Jul 2019 10:03:12	U	SMPL
K3158-09MSD - 1	OK-01-062819MSD	25258	4.7512	-7471B	PPB	PPB	02 Jul 2019 10:05:30	U	SMPL
K3160-07 - 1	EO-01-062819-A	27434	5.1595	-7471B	PPB	PPB	02 Jul 2019 10:07:46	U	SMPL
CCV70 - 1	CCV70	27194	5.1145	-7471B	PPB	PPB	02 Jul 2019 10:10:02	U	SMPL
CCB70 - 1	CCB70	-107	-0.0086	-7471B	PPB	PPB	02 Jul 2019 10:12:19	U	SMPL
K3160-09 - 1	EO-01-062819-B	17241	3.2468	-7471B	PPB	PPB	02 Jul 2019 10:14:35	U	SMPL
K3160-11 - 1	EO-01-062819-C	5642	1.0702	-7471B	PPB	PPB	02 Jul 2019 10:16:52	U	SMPL
K3592-01 - 1	RT-5124	2132	0.4116	-7471B	PPB	PPB	02 Jul 2019 10:19:08	U	SMPL
K3592-03 - 1	RBR-200052	1514	0.2956	-7471B	PPB	PPB	02 Jul 2019 10:21:24	U	SMPL
K3601-01 - 1	RT-4651	2194	0.4232	-7471B	PPB	PPB	02 Jul 2019 10:23:40	U	SMPL
K3601-03 - 1	RBR-200027	2099	0.4054	-7471B	PPB	PPB	02 Jul 2019 10:25:58	U	SMPL
K3606-02 - 1	HJDC-COMP-1	16670	3.1396	-7471B	PPB	PPB	02 Jul 2019 10:28:15	U	SMPL
K3628-01 - 1	VNJ-217-368	-71	-0.0018	-7471B	PPB	PPB	02 Jul 2019 10:30:33	U	SMPL
K3628-03 - 1	VNJ-226-VNJ-238	-46	0.0029	-7471B	PPB	PPB	02 Jul 2019 10:32:51	U	SMPL
K3628-05 - 1	VNJ-231-VNJ-236-345	-38	0.0044	-7471B	PPB	PPB	02 Jul 2019 10:35:07	U	SMPL
CCV71 - 1	CCV71	27208	5.1171	-7471B	PPB	PPB	02 Jul 2019 10:37:23	U	SMPL
CCB71 - 1	CCB71	-115	-0.0101	-7471B	PPB	PPB	02 Jul 2019 10:39:39	U	SMPL
K3628-07 - 1	DRUM-COMP	195	0.0481	-7471B	PPB	PPB	02 Jul 2019 10:41:55	U	SMPL
K3629-01 - 1	NB-SOIL-PILE	1381	0.2707	-7471B	PPB	PPB	02 Jul 2019 10:44:11	U	SMPL
K3634-02 - 1	HJOC-COMP-2	14527	2.7375	-7471B	PPB	PPB	02 Jul 2019 10:46:27	U	SMPL
K3158-09LX5 - 1		628	0.1294	-7471B	PPB	PPB	02 Jul 2019 10:48:43	U	SMPL
K3158-09A - 1		26253	4.9379	-7471B	PPB	PPB	02 Jul 2019 10:50:59	U	SMPL
CCV72 - 1	CCV72	26975	5.0734	-7471B	PPB	PPB	02 Jul 2019 10:53:16	U	SMPL
CCB72 - 1	CCB72	-151	-0.0168	-7471B	PPB	PPB	02 Jul 2019 10:55:34	U	SMPL