


LB103834

7471B

INSTRUMENT ID: CU1

Linear

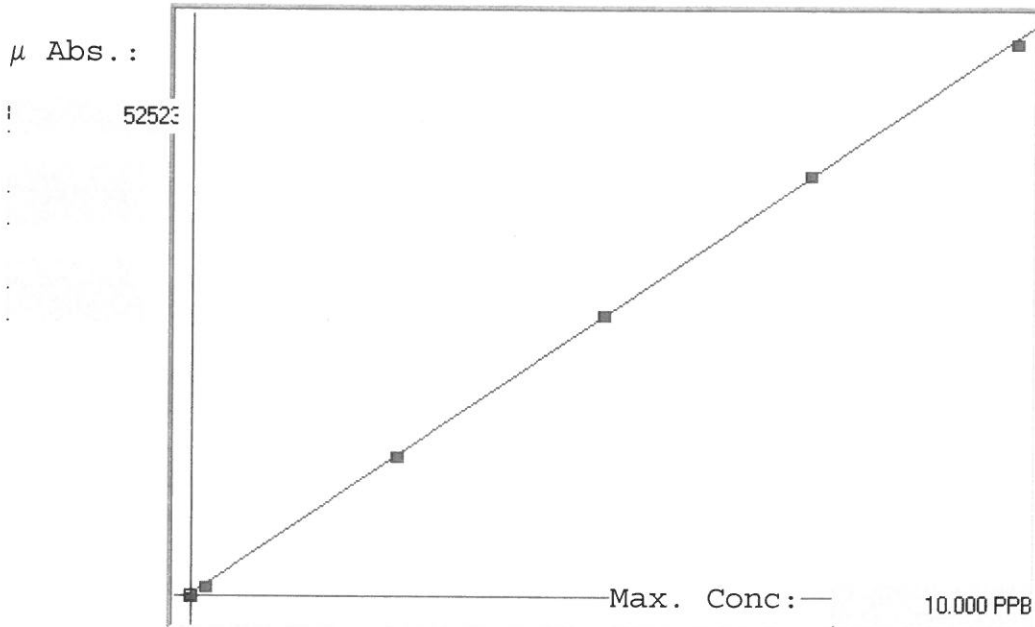

A= 0.0000e+000

B= 1.8927e-004

C= -1.8474e-002

Rho= 0.9999136

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.013	-0.013	27	0.000	27				
0.2	0.200	0.170	-0.030	994	0.0 %	994				
2.5	2.500	2.509	0.009	13353	0.0 %	13353				
5.0	5.000	5.039	0.039	26722	0.0 %	26722				
7.5	7.500	7.573	0.073	40112	0.0 %	40112				
10.0	10.000	9.922	-0.078	52523	0.0 %	52523				

LB103834 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 08 Jul 2019 13:34:26

Sample ID	Extended ID	µ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50.0	27	-	0.00007471B	PPB	08 Jul 2019 13:36:37	S	Std
0.2 - 1	50.2	994	-	0.20007471B	PPB	08 Jul 2019 13:38:55	S	Std
2.5 - 1	52.5	13353	-	2.50007471B	PPB	08 Jul 2019 13:41:13	S	Std
5.0 - 1	55.0	26722	-	5.00007471B	PPB	08 Jul 2019 13:43:30	S	Std
7.5 - 1	57.5	40112	-	7.50007471B	PPB	08 Jul 2019 13:45:47	S	Std
10.0 - 1	57.0	52523	-	10.00007471B	PPB	08 Jul 2019 13:54:05	S	Std
ICV22 - 1	ICV22	21687	4.0862	-7471B	PPB	08 Jul 2019 13:58:01	U	SMPL
ICB22 - 1	ICB22	-76	-0.0329	-7471B	PPB	08 Jul 2019 14:00:17	U	SMPL
CCV91 - 1	CCV91	26882	5.0694	-7471B	PPB	08 Jul 2019 14:02:33	U	SMPL
CCB91 - 1	CCB91	-69	-0.0315	-7471B	PPB	08 Jul 2019 14:04:48	U	SMPL
CRA - 1	CRA	1065	0.1831	-7471B	PPB	08 Jul 2019 14:07:06	U	SMPL
HighStd - 1	HighStd	53845	10.1726	-7471B	PPB	08 Jul 2019 14:09:22	U	SMPL
ChkStd - 1	ChkStd	37451	7.0698	-7471B	PPB	08 Jul 2019 14:11:41	U	SMPL
PB121215BL - 1	PBS	180	0.0156	-7471B	PPB	08 Jul 2019 14:14:03	U	SMPL
PB121215BS - 1	LCSS	21807	4.1089	-7471B	PPB	08 Jul 2019 14:16:23	U	SMPL
K3622-01 - 1	OR-02-070319-A	2062	0.3718	-7471B	PPB	08 Jul 2019 14:18:42	U	SMPL
K3622-03 - 1	OR-02-070319-B	2719	0.4961	-7471B	PPB	08 Jul 2019 14:21:01	U	SMPL
K3624-01 - 1	PL-01-070319-A	1159	0.2009	-7471B	PPB	08 Jul 2019 14:23:19	U	SMPL
K3624-03 - 1	PL-01-070319-B	1420	0.2503	-7471B	PPB	08 Jul 2019 14:25:36	U	SMPL
K3624-05 - 1	PL-01-070319-C	1615	0.2872	-7471B	PPB	08 Jul 2019 14:27:52	U	SMPL
CCV92 - 1	CCV92	27232	5.1356	-7471B	PPB	08 Jul 2019 14:30:08	U	SMPL
CCB92 - 1	CCB92	-26	-0.0234	-7471B	PPB	08 Jul 2019 14:32:24	U	SMPL
K3624-07 - 1	PL-01-070319-D	1550	0.2749	-7471B	PPB	08 Jul 2019 14:34:41	U	SMPL
K3668-01 - 1	TRANSFORMER-1	5146	0.9555	-7471B	PPB	08 Jul 2019 14:36:56	U	SMPL
K3668-05 - 1	SHORT-WALL-AREA	2904	0.5312	-7471B	PPB	08 Jul 2019 14:39:12	U	SMPL
K3668-09 - 1	TRANSFORMER-T2	645	0.1036	-7471B	PPB	08 Jul 2019 14:41:28	U	SMPL
K3681-01 - 1	PILEA-07-01-19	2360	0.4282	-7471B	PPB	08 Jul 2019 14:43:45	U	SMPL
K3681-02 - 1	TOP-SOIL-07-01-19	7396	1.3813	-7471B	PPB	08 Jul 2019 14:46:02	U	SMPL
K3681-03 - 1	STOCK-PILE-07-01-19	5929	1.1037	-7471B	PPB	08 Jul 2019 14:48:19	U	SMPL
K3682-01 - 1	D-2-ROLL-OFF-2-STOCK-PILE	618	0.0985	-7471B	PPB	08 Jul 2019 14:50:37	U	SMPL
K3682-01DUP - 1	D-2-ROLL-OFF-2-STOCK-PILEDUP	601	0.0953	-7471B	PPB	08 Jul 2019 14:52:55	U	SMPL
K3682-01MS - 1	D-2-ROLL-OFF-2-STOCK-PILEMS	18278	3.4409	-7471B	PPB	08 Jul 2019 14:55:11	U	SMPL
CCV93 - 1	CCV93	27045	5.1002	-7471B	PPB	08 Jul 2019 14:57:27	U	SMPL
CCB93 - 1	CCB93	229	0.0249	-7471B	PPB	08 Jul 2019 14:59:44	U	SMPL
K3682-01MSD - 1	D-2-ROLL-OFF-2-STOCK-PILEMSD	17804	3.3512	-7471B	PPB	08 Jul 2019 15:02:01	U	SMPL
K3682-01LX5 - 1		215	0.0222	-7471B	PPB	08 Jul 2019 15:04:18	U	SMPL
K3682-01A - 1		18272	3.4398	-7471B	PPB	08 Jul 2019 15:06:34	U	SMPL
CCV94 - 1	CCV94	27204	5.1303	-7471B	PPB	08 Jul 2019 15:08:51	U	SMPL
CCB94 - 1	CCB94	92	-0.0011	-7471B	PPB	08 Jul 2019 15:11:08	U	SMPL