


LB103837

7470A

INSTRUMENT ID: CU1

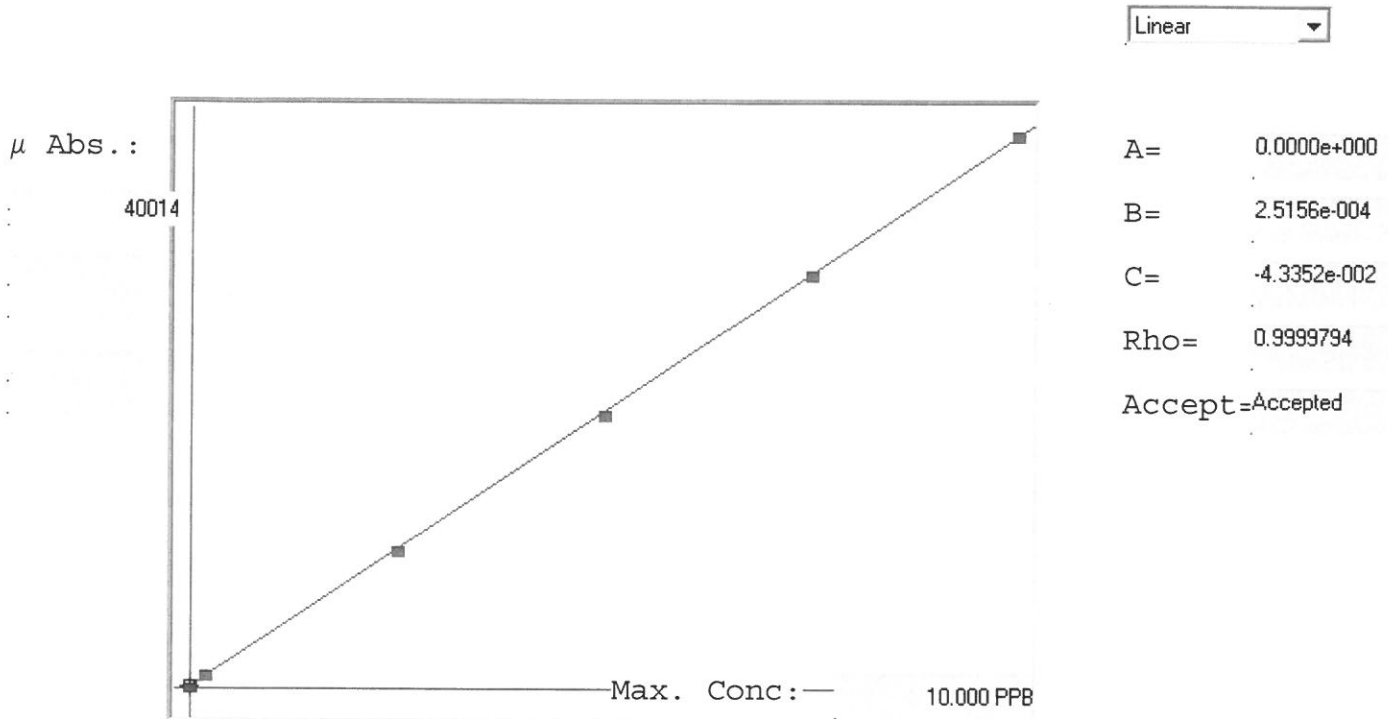

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.001	-0.001	170	0.000	170				
0.2	0.200	0.234	0.034	1103	0.0 %	1103				
2.5	2.500	2.481	-0.019	10036	0.0 %	10036				
5.0	5.000	4.963	-0.037	19903	0.0 %	19903				
7.5	7.500	7.499	-0.001	29984	0.0 %	29984				
10.0	10.000	10.022	0.022	40014	0.0 %	40014				

LB103837 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 08 Jul 2019 15:38:56

Sample ID	Extended ID	μ Abs	Conc	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50.0	170	-	0.00007470A	PPB	08 Jul 2019 15:42:19	S	Std
0.2 - 1	50.2	1103	-	0.20007470A	PPB	08 Jul 2019 15:44:29	S	Std
2.5 - 1	52.5	10036	-	2.50007470A	PPB	08 Jul 2019 15:46:37	S	Std
5.0 - 1	55.0	19903	-	5.00007470A	PPB	08 Jul 2019 15:48:46	S	Std
7.5 - 1	57.5	29984	-	7.50007470A	PPB	08 Jul 2019 15:50:56	S	Std
10.0 - 1	510.0	40014	-	10.00007470A	PPB	08 Jul 2019 15:53:03	S	Std
ICV23 - 1	ICV23	15890	3.9539	-7470A	PPB	08 Jul 2019 15:58:37	U	SMPL
ICB23 - 1	ICB23	111	-0.0154	-7470A	PPB	08 Jul 2019 16:00:43	U	SMPL
CCV95 - 1	CCV95	19622	4.8927	-7470A	PPB	08 Jul 2019 16:02:50	U	SMPL
CCB95 - 1	CCB95	107	-0.0164	-7470A	PPB	08 Jul 2019 16:04:57	U	SMPL
CRA - 1	CRA	1061	0.2236	-7470A	PPB	08 Jul 2019 16:07:04	U	SMPL
HighStd - 1	HighStd	40096	10.0431	-7470A	PPB	08 Jul 2019 16:09:11	U	SMPL
ChkStd - 1	ChkStd	28091	7.0231	-7470A	PPB	08 Jul 2019 16:11:18	U	SMPL
PB121216BL - 1	PBW	64	-0.0273	-7470A	PPB	08 Jul 2019 16:13:25	U	SMPL
PB121216BS - 1	LCSW	15076	3.7491	-7470A	PPB	08 Jul 2019 16:15:34	U	SMPL
K3622-02 - 1	OR-02-070319-A	104	-0.0172	-7470A	PPB	08 Jul 2019 16:17:41	U	SMPL
K3622-02DUP - 1	OR-02-070319-ADUP	129	-0.0109	-7470A	PPB	08 Jul 2019 16:19:50	U	SMPL
K3622-02MS - 1	OR-02-070319-AMS	16144	4.0178	-7470A	PPB	08 Jul 2019 16:21:58	U	SMPL
K3622-02MSD - 1	OR-02-070319-AMSD	17257	4.2978	-7470A	PPB	08 Jul 2019 16:24:07	U	SMPL
K3622-04 - 1	OR-02-070319-B	260	0.0221	-7470A	PPB	08 Jul 2019 16:26:14	U	SMPL
CCV96 - 1	CCV96	19603	4.8879	-7470A	PPB	08 Jul 2019 16:28:20	U	SMPL
CCB96 - 1	CCB96	84	-0.0222	-7470A	PPB	08 Jul 2019 16:30:27	U	SMPL
K3624-02 - 1	PL-01-070319-A	373	0.0505	-7470A	PPB	08 Jul 2019 16:32:34	U	SMPL
K3624-04 - 1	PL-01-070319-B	134	-0.0096	-7470A	PPB	08 Jul 2019 16:34:41	U	SMPL
K3624-06 - 1	PL-01-070319-C	169	-0.0008	-7470A	PPB	08 Jul 2019 16:36:48	U	SMPL
K3624-08 - 1	PL-01-070319-D	162	-0.0026	-7470A	PPB	08 Jul 2019 16:38:55	U	SMPL
K3668-04 - 1	TRANSFORMER-1	192	0.0049	-7470A	PPB	08 Jul 2019 16:41:03	U	SMPL
K3668-08 - 1	SHORT-WALL-AREA	269	0.0243	-7470A	PPB	08 Jul 2019 16:43:10	U	SMPL
K3668-12 - 1	TRANSFORMER-T2	355	0.0460	-7470A	PPB	08 Jul 2019 16:45:18	U	SMPL
K3682-03 - 1	D-2-ROLL-OFF-2-STOCK-PILE	146	-0.0066	-7470A	PPB	08 Jul 2019 16:47:26	U	SMPL
PB121216TB - 1	PB121168TB	168	-0.0011	-7470A	PPB	08 Jul 2019 16:49:35	U	SMPL
K3622-02LX5 - 1		52	-0.0303	-7470A	PPB	08 Jul 2019 16:51:42	U	SMPL
CCV97 - 1	CCV97	19360	4.8268	-7470A	PPB	08 Jul 2019 16:53:49	U	SMPL
CCB97 - 1	CCB97	83	-0.0225	-7470A	PPB	08 Jul 2019 16:55:55	U	SMPL
K3622-02A - 1		16546	4.1189	-7470A	PPB	08 Jul 2019 16:58:02	U	SMPL
CCV98 - 1	CCV98	19091	4.7591	-7470A	PPB	08 Jul 2019 17:00:09	U	SMPL
CCB98 - 1	CCB98	99	-0.0184	-7470A	PPB	08 Jul 2019 17:02:15	U	SMPL