


LB103870

7470A

INSTRUMENT ID: CV1

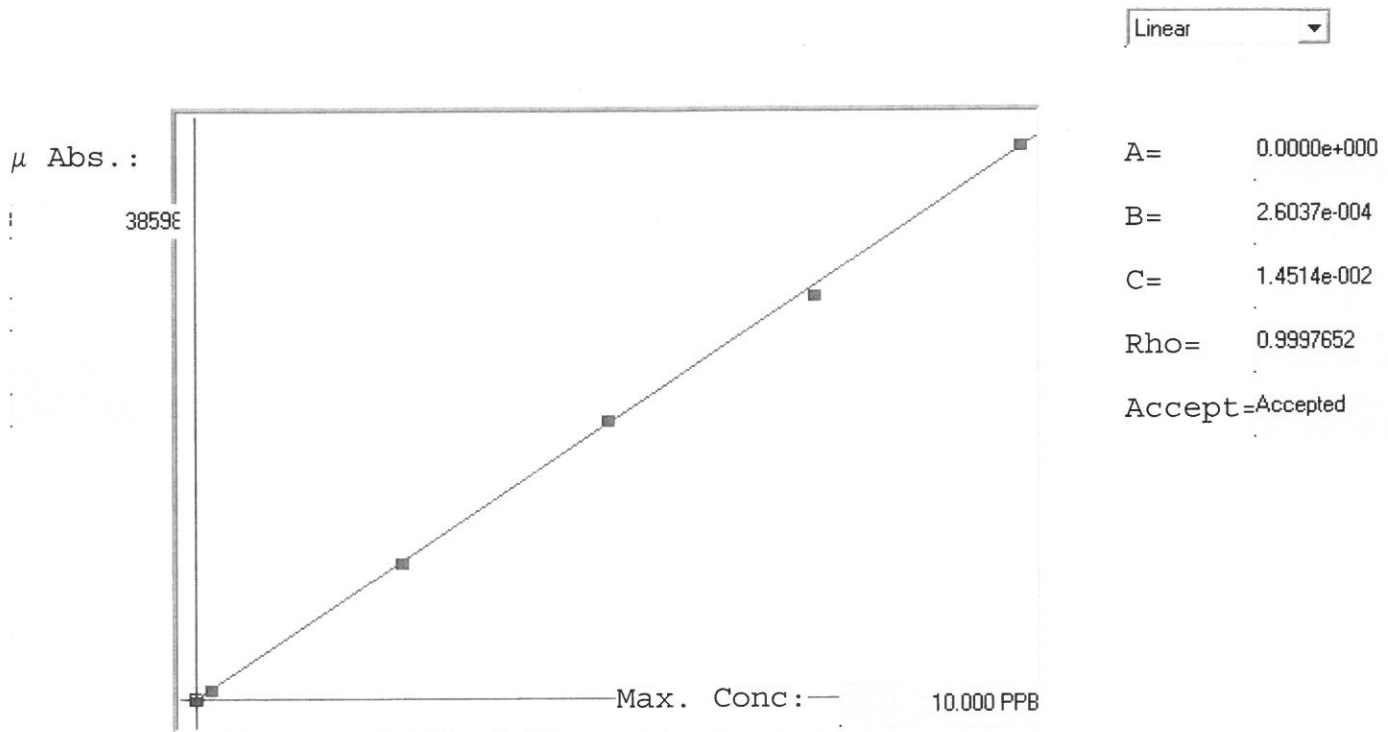

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.011	-0.011	-98	0.000	-98				
0.2	0.200	0.202	0.002	720	0.0 %	720				
2.5	2.500	2.505	0.005	9565	0.0 %	9565				
5.0	5.000	5.097	0.097	19520	0.0 %	19520				
7.5	7.500	7.343	-0.157	28146	0.0 %	28146				
10.0	10.000	10.064	0.064	38598	0.0 %	38598				

LB103870 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 10 Jul 2019 10:49:06				
Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type
0.0 - 1	50.0	-98	-	0.00007470A	PPB		10 Jul 2019 11:34:49	S Std
0.2 - 1	50.2	720	-	0.20007470A	PPB		10 Jul 2019 11:36:58	S Std
2.5 - 1	52.5	9565	-	2.50007470A	PPB		10 Jul 2019 11:39:07	S Std
5.0 - 1	55.0	19520	-	5.00007470A	PPB		10 Jul 2019 11:41:15	S Std
7.5 - 1	57.5	28146	-	7.50007470A	PPB		10 Jul 2019 11:43:23	S Std
10.0 - 1	510.0	38598	-	10.00007470A	PPB		10 Jul 2019 11:45:31	S Std
ICV27 - 1	ICV27	15199	3.9719	-7470A	PPB		10 Jul 2019 11:52:50	U SMPL
ICB27 - 1	ICB27	-16	0.0103	-7470A	PPB		10 Jul 2019 11:54:57	U SMPL
CCV06 - 1	CCV06	18925	4.9420	-7470A	PPB		10 Jul 2019 11:57:03	U SMPL
CCB06 - 1	CCB06	-43	0.0033	-7470A	PPB		10 Jul 2019 11:59:09	U SMPL
CRA - 1	CRA	694	0.1952	-7470A	PPB		10 Jul 2019 12:01:16	U SMPL
HighStd - 1	HighStd	36194	9.4383	-7470A	PPB		10 Jul 2019 12:03:23	U SMPL
ChkStd - 1	ChkStd	25732	6.7143	-7470A	PPB		10 Jul 2019 12:05:30	U SMPL
PB121257BL - 1	PBW	-67	-0.0029	-7470A	PPB		10 Jul 2019 12:07:38	U SMPL
PB121257BS - 1	LCSW	15283	3.9937	-7470A	PPB		10 Jul 2019 12:09:46	U SMPL
K3627-02 - 1	TR-05-070819	4	0.0156	-7470A	PPB		10 Jul 2019 12:11:53	U SMPL
K3627-02DUP - 1	TR-05-070819DUP	13	0.0179	-7470A	PPB		10 Jul 2019 12:14:01	U SMPL
K3627-02MS - 1	TR-05-070819MS	15760	4.1179	-7470A	PPB		10 Jul 2019 12:16:09	U SMPL
K3627-02MSD - 1	TR-05-070819MSD	15152	3.9596	-7470A	PPB		10 Jul 2019 12:18:17	U SMPL
K3687-07 - 1	72-12017-VNJ-206	-10	0.0119	-7470A	PPB		10 Jul 2019 12:20:24	U SMPL
CCV07 - 1	CCV07	19070	4.9798	-7470A	PPB		10 Jul 2019 12:22:31	U SMPL
CCB07 - 1	CCB07	-29	0.0070	-7470A	PPB		10 Jul 2019 12:24:38	U SMPL
K3687-08 - 1	CONCRETE-RBR-251685	11	0.0174	-7470A	PPB		10 Jul 2019 12:26:44	U SMPL
K3693-02 - 1	RBR-200028	2	0.0150	-7470A	PPB		10 Jul 2019 12:28:51	U SMPL
K3694-08 - 1	GC-SOIL-PILE	0	0.0145	-7470A	PPB		10 Jul 2019 12:30:59	U SMPL
K3695-01 - 1	SOIL-SAMPLE-1	8	0.0166	-7470A	PPB		10 Jul 2019 12:33:06	U SMPL
K3695-02 - 1	SOIL-SAMPLE-2	32	0.0228	-7470A	PPB		10 Jul 2019 12:35:14	U SMPL
K3695-03 - 1	SOIL-SAMPLE-3	40	0.0249	-7470A	PPB		10 Jul 2019 12:37:22	U SMPL
K3697-03 - 1	72-12000	14	0.0182	-7470A	PPB		10 Jul 2019 12:39:30	U SMPL
K3697-06 - 1	RBR-200035	-5	0.0132	-7470A	PPB		10 Jul 2019 12:41:38	U SMPL
PB121258BL - 1	PBW	-8	0.0124	-7470A	PPB		10 Jul 2019 12:43:46	U SMPL
PB121258BS - 1	LCSW	15310	4.0008	-7470A	PPB		10 Jul 2019 12:45:53	U SMPL
CCV08 - 1	CCV08	19063	4.9779	-7470A	PPB		10 Jul 2019 12:48:00	U SMPL
CCB08 - 1	CCB08	-14	0.0109	-7470A	PPB		10 Jul 2019 12:50:07	U SMPL
K3712-02 - 1	TT-003-IDWGW-20190708	469	0.1366	-7470A	PPB		10 Jul 2019 12:52:13	U SMPL
K3712-03 - 1	TT-004-IDWGW-20190708	547	0.1569	-7470A	PPB		10 Jul 2019 12:54:20	U SMPL
K3712-03DUP - 1	TT-004-IDWGW-20190708DUP	544	0.1562	-7470A	PPB		10 Jul 2019 12:56:26	U SMPL
K3712-03MS - 1	TT-004-IDWGW-20190708MS	16805	4.3900	-7470A	PPB		10 Jul 2019 12:58:33	U SMPL
K3712-03MSD - 1	TT-004-IDWGW-20190708MSD	16831	4.3968	-7470A	PPB		10 Jul 2019 13:00:40	U SMPL
PB121257TB - 1	PB121212TB	-25	0.0080	-7470A	PPB		10 Jul 2019 13:02:47	U SMPL
K3627-02LX5 - 1		16	0.0187	-7470A	PPB		10 Jul 2019 13:04:55	U SMPL
K3627-02A - 1		15528	4.0575	-7470A	PPB		10 Jul 2019 13:07:03	U SMPL
K3712-03LX5 - 1		69	0.0325	-7470A	PPB		10 Jul 2019 13:09:11	U SMPL
K3712-03A - 1		16988	4.4377	-7470A	PPB		10 Jul 2019 13:11:19	U SMPL
CCV09 - 1	CCV09	18824	4.9157	-7470A	PPB		10 Jul 2019 13:13:26	U SMPL
CCB09 - 1	CCB09	-39	0.0044	-7470A	PPB		10 Jul 2019 13:15:32	U SMPL