

LB103873

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

7/10/2019 11:02

Test: Total CN

Sample Id	Result <i>ug/d</i>	Dil. 1 +	Response	Errors
ICV1	97.935	0.0	0.096	
ICB1	0.882	0.0	0.002	
CCV1	244.753	0.0	0.238	
CCB1	0.314	0.0	0.001	
PB121199BL	0.631	0.0	0.001	
PB121199BS	99.345	0.0	0.097	
MIDPB121199	244.920	0.0	0.238	
K3591-10	1.873	0.0	0.003	
K3666-02	7.231	0.0	0.008	
K3666-02DUP	7.588	0.0	0.008	
K3666-02MS	42.372	0.0	0.042	
K3666-02MSD	44.398	0.0	0.044	
K3691-11	4.059	0.0	0.005	
CCV2	256.969	0.0	0.250	
CCB2	0.397	0.0	0.001	

N	15
Mean	70.244
SD	98.2950
CV%	139.93

Aquakem v. 7.2AQ1

Results from time period:

Wed Jul 10 10:51:45 2019

Wed Jul 10 10:57:05 2019

AS

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.5796	µg/l	7/10/2019 9:23:47	
5.0PPBCN	A	Total CN	P	4.7786	µg/l	7/10/2019 9:23:48	
10PPBCN	A	Total CN	P	10.0545	µg/l	7/10/2019 9:23:49	
50PPBCN	A	Total CN	P	50.0476	µg/l	7/10/2019 9:23:50	
100PPBCN	A	Total CN	P	100.425	µg/l	7/10/2019 9:23:51	
250PPBCN	A	Total CN	P	248.4064	µg/l	7/10/2019 9:23:52	
500PPBCN	A	Total CN	P	500.7082	µg/l	7/10/2019 9:23:53	
ICV1	S	Total CN	P	97.9345	µg/l	7/10/2019 10:51:45	
ICB1	S	Total CN	P	0.8822	µg/l	7/10/2019 10:51:46	
CCV1	S	Total CN	P	244.7525	µg/l	7/10/2019 10:51:47	
CCB1	S	Total CN	P	0.3142	µg/l	7/10/2019 10:51:48	
PB121199BL	S	Total CN	P	0.6307	µg/l	7/10/2019 10:51:49	
PB121199BS	S	Total CN	P	99.3452	µg/l	7/10/2019 10:51:50	
MIDPB121199	S	Total CN	P	244.9201	µg/l	7/10/2019 10:51:51	
K3591-10	S	Total CN	P	1.873	µg/l	7/10/2019 10:51:52	
K3666-02	S	Total CN	P	7.2308	µg/l	7/10/2019 10:51:53	
K3666-02DUP	S	Total CN	P	7.5877	µg/l	7/10/2019 10:51:54	
K3666-02MS	S	Total CN	P	42.3724	µg/l	7/10/2019 10:51:55	
K3666-02MSD	S	Total CN	P	44.3983	µg/l	7/10/2019 10:57:00	
K3691-11	S	Total CN	P	4.0595	µg/l	7/10/2019 10:57:01	
CCV2	S	Total CN	P	256.9686	µg/l	7/10/2019 10:57:04	
CCB2	S	Total CN	P	0.3974	µg/l	7/10/2019 10:57:05	

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AS

Instrument ID : Konelab

7/10/2019 9:31


Test Total CN

Accepted 7/10/2019 9:31

Factor 1031
 Bias 0.001

Coeff. of det. 0.999982

Errors

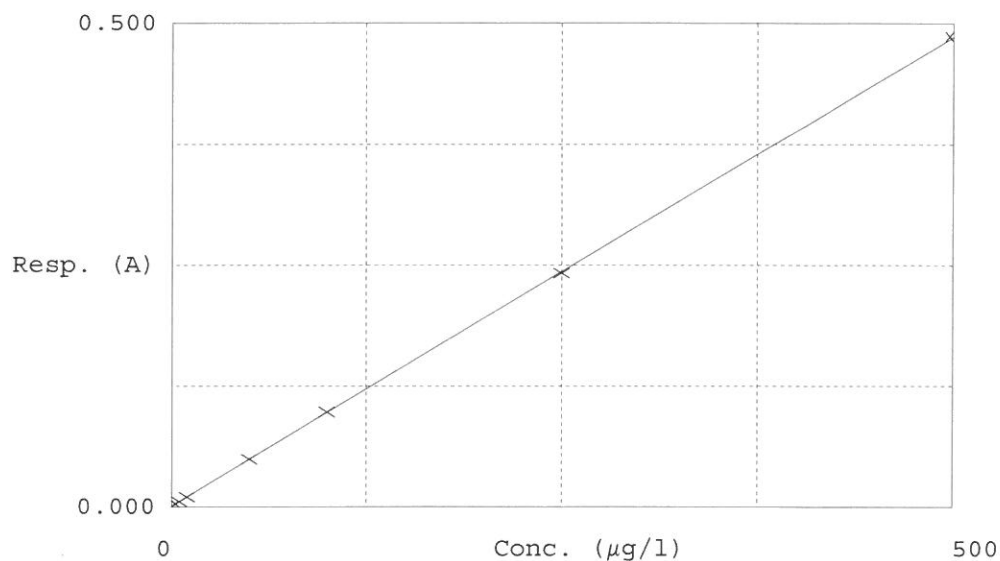

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.5796	0.0000	
2	5.0PPBCN	0.005	4.7786	5.0000	
3	10PPBCN	0.010	10.0545	10.0000	
4	50PPBCN	0.049	50.0476	50.0000	
5	100PPBCN	0.098	100.4250	100.0000	
6	250PPBCN	0.242	248.4064	250.0000	
7	500PPBCN	0.487	500.7082	500.0000	