


LB103882

7471B

INSTRUMENT ID : CU1

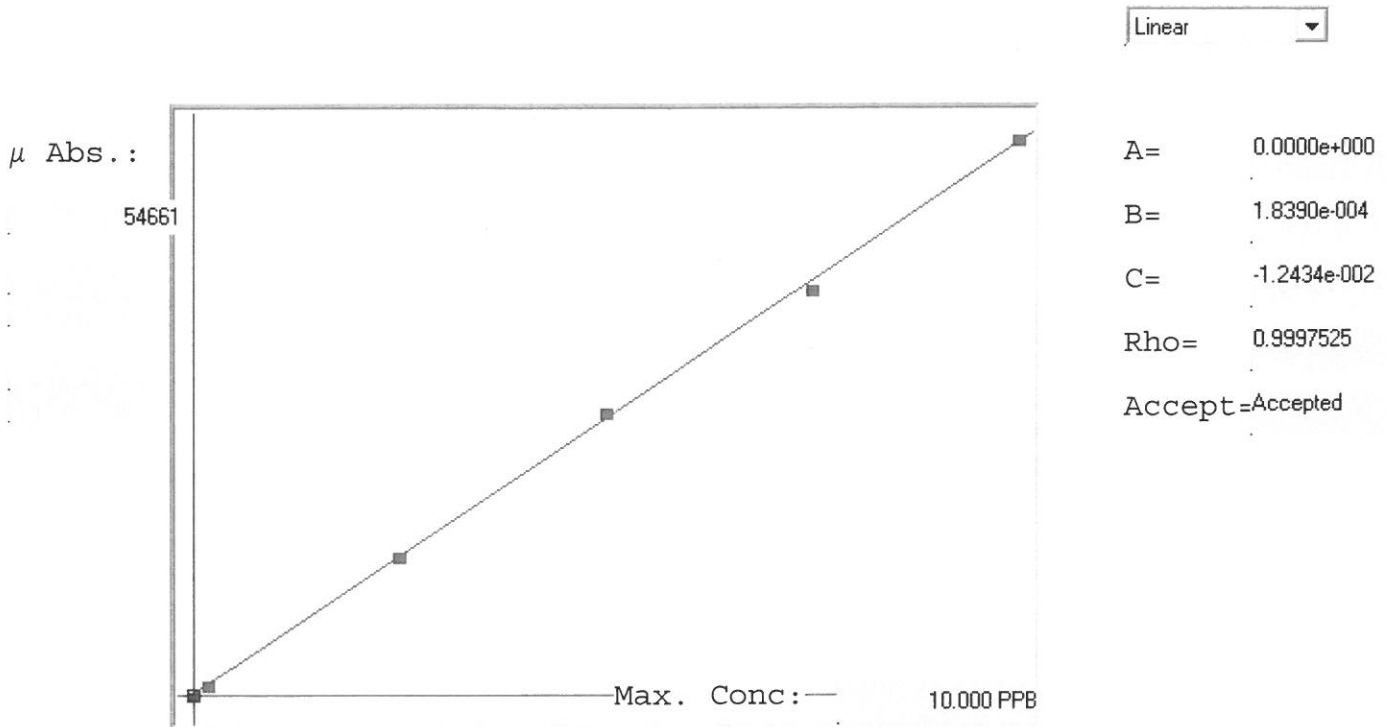

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.002	-0.002	58	0.000	58				
0.2	0.200	0.164	-0.036	960	0.0 %	960				
2.5	2.500	2.521	0.021	13774	0.0 %	13774				
5.0	5.000	5.125	0.125	27935	0.0 %	27935				
7.5	7.500	7.353	-0.147	40052	0.0 %	40052				
10.0	10.000	10.039	0.039	54661	0.0 %	54661				

LB103882 INSTRUMENT ID : CV1

Method: 7471B	Operator: Admin	Date of Analysis: 10 Jul 2019 14:15:10							
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	58	-	0.0000	7471B	PPB	10 Jul 2019 14:18:49	S	Std
0.2 - 1	50-2	960	-	0.2000	7471B	PPB	10 Jul 2019 14:21:07	S	Std
2.5 - 1	52-5	13774	-	2.5000	7471B	PPB	10 Jul 2019 14:23:26	S	Std
5.0 - 1	55-0	27935	-	5.0000	7471B	PPB	10 Jul 2019 14:25:43	S	Std
7.5 - 1	57-5	40052	-	7.5000	7471B	PPB	10 Jul 2019 14:28:00	S	Std
10.0 - 1	510-0	54661	-	10.0000	7471B	PPB	10 Jul 2019 14:30:18	S	Std
ICV28 - 1	ICV28	22157	4.0621	-	7471B	PPB	10 Jul 2019 14:34:08	U	SMPL
ICB28 - 1	ICB28	35	-0.0060	-	7471B	PPB	10 Jul 2019 14:36:23	U	SMPL
CCV10 - 1	CCV10	27791	5.0982	-	7471B	PPB	10 Jul 2019 14:38:39	U	SMPL
CCB10 - 1	CCB10	9	-0.0108	-	7471B	PPB	10 Jul 2019 14:40:54	U	SMPL
CRA - 1	CRA	947	0.1617	-	7471B	PPB	10 Jul 2019 14:43:11	U	SMPL
HighStd - 1	HighStd	54539	10.0170	-	7471B	PPB	10 Jul 2019 14:45:26	U	SMPL
ChkStd - 1	ChkStd	37285	6.8441	-	7471B	PPB	10 Jul 2019 14:47:42	U	SMPL
PB121273BL - 1	PBS	-42	-0.0202	-	7471B	PPB	10 Jul 2019 14:50:00	U	SMPL
PB121273BS - 1	LCSS	22287	4.0860	-	7471B	PPB	10 Jul 2019 14:52:18	U	SMPL
K3626-01 - 1	SU-02-070919-A	1442	0.2527	-	7471B	PPB	10 Jul 2019 14:54:35	U	SMPL
K3626-01DUP - 1	SU-02-070919-ADUP	1229	0.2136	-	7471B	PPB	10 Jul 2019 14:56:53	U	SMPL
K3626-01MS - 1	SU-02-070919-AMS	20289	3.7186	-	7471B	PPB	10 Jul 2019 14:59:10	U	SMPL
K3626-01MSD - 1	SU-02-070919-AMSD	21440	3.9303	-	7471B	PPB	10 Jul 2019 15:01:28	U	SMPL
K3626-03 - 1	SU-02-070919-B	683	0.1132	-	7471B	PPB	10 Jul 2019 15:03:45	U	SMPL
CCV11 - 1	CCV11	27474	5.0399	-	7471B	PPB	10 Jul 2019 15:06:05	U	SMPL
CCB11 - 1	CCB11	20	-0.0088	-	7471B	PPB	10 Jul 2019 15:08:22	U	SMPL
K3716-01 - 1	CONCRETE-1	670	0.1108	-	7471B	PPB	10 Jul 2019 15:10:39	U	SMPL
K3716-02 - 1	CONCRETE-2	250	0.0335	-	7471B	PPB	10 Jul 2019 15:12:55	U	SMPL
K3716-03 - 1	CONCRETE-3	148	0.0148	-	7471B	PPB	10 Jul 2019 15:15:12	U	SMPL
K3716-04 - 1	WHITE-BLOCK	3978	0.7191	-	7471B	PPB	10 Jul 2019 15:17:29	U	SMPL
K3716-05 - 1	BLUE-BLOCK	36574	6.7134	-	7471B	PPB	10 Jul 2019 15:19:46	U	SMPL
K3716-06 - 1	RECTANGULAR-BLOCK	130	0.0115	-	7471B	PPB	10 Jul 2019 15:22:03	U	SMPL
K3716-07 - 1	SQUARE-BLOCK	221	0.0282	-	7471B	PPB	10 Jul 2019 15:24:20	U	SMPL
K3626-01LX5 - 1		230	0.0299	-	7471B	PPB	10 Jul 2019 15:26:37	U	SMPL
K3626-01A - 1		20909	3.8326	-	7471B	PPB	10 Jul 2019 15:28:55	U	SMPL
CCV12 - 1	CCV12	27414	5.0289	-	7471B	PPB	10 Jul 2019 15:31:11	U	SMPL
CCB12 - 1	CCB12	15	-0.0097	-	7471B	PPB	10 Jul 2019 15:33:28	U	SMPL