


LB103909

7471B

INSTRUMENT ID: CV1

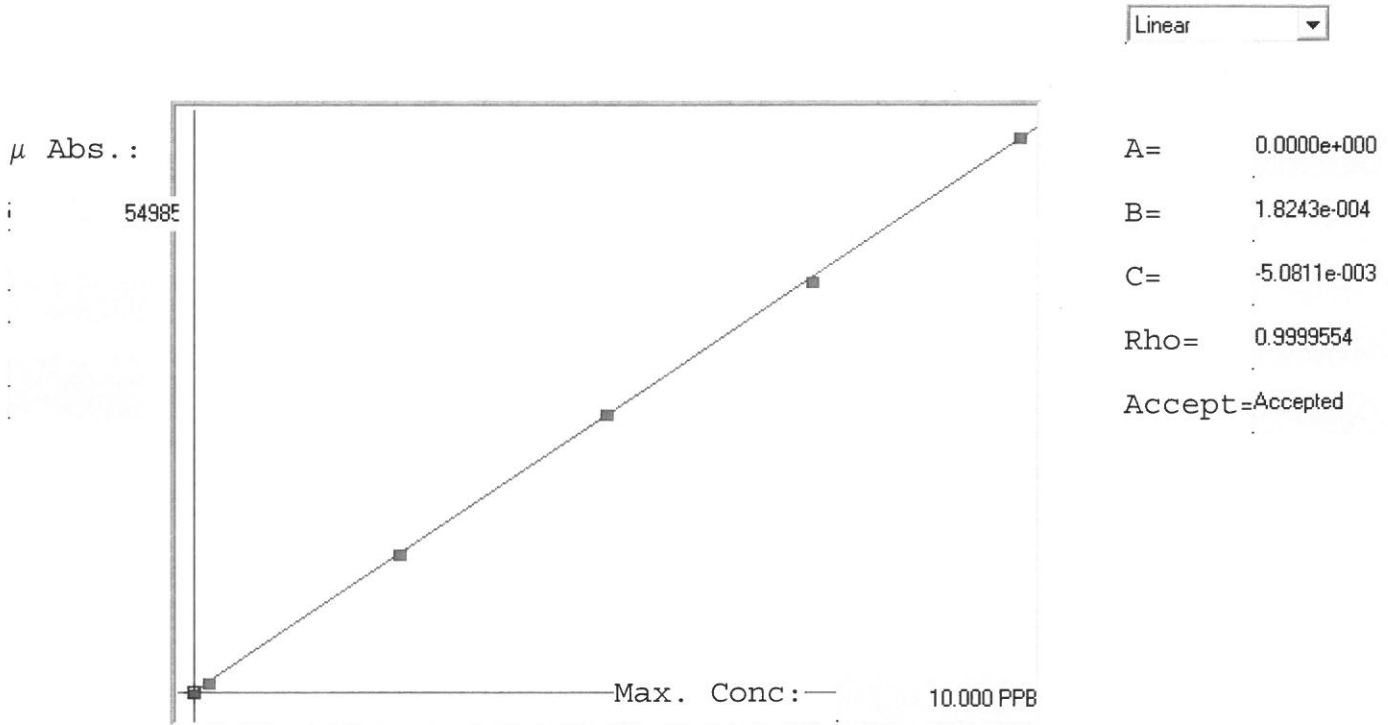

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.005	0.005	56	0.000	56				
0.2	0.200	0.180	-0.020	1014	0.0 %	1014				
2.5	2.500	2.516	0.016	13821	0.0 %	13821				
5.0	5.000	5.039	0.039	27652	0.0 %	27652				
7.5	7.500	7.434	-0.066	40777	0.0 %	40777				
10.0	10.000	10.026	0.026	54985	0.0 %	54985				

LB103909 INSTRUMENT ID : CV1

Method: 7471B	Operator: Admin	Date of Analysis: 11 Jul 2019 14:03:04							
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	56	-	0.00007471B		PPB	11 Jul 2019 14:06:56	S	Std
0.2 - 1	50-2	1014	-	0.20007471B		PPB	11 Jul 2019 14:09:15	S	Std
2.5 - 1	52-5	13821	-	2.50007471B		PPB	11 Jul 2019 14:11:33	S	Std
5.0 - 1	55-0	27652	-	5.00007471B		PPB	11 Jul 2019 14:13:52	S	Std
7.5 - 1	57-5	40777	-	7.50007471B		PPB	11 Jul 2019 14:16:09	S	Std
10.0 - 1	510-0	54985	-	10.00007471B		PPB	11 Jul 2019 14:18:26	S	Std
ICV30 - 1	ICV30	22366	4.0751	-7471B		PPB	11 Jul 2019 14:22:42	U	SMPL
ICB30 - 1	ICB30	-33	-0.0111	-7471B		PPB	11 Jul 2019 14:24:59	U	SMPL
CCV16 - 1	CCV16	27505	5.0126	-7471B		PPB	11 Jul 2019 14:27:15	U	SMPL
CCB16 - 1	CCB16	14	-0.0025	-7471B		PPB	11 Jul 2019 14:29:30	U	SMPL
CRA - 1	CRA	997	0.1768	-7471B		PPB	11 Jul 2019 14:31:47	U	SMPL
HighStd - 1	HighStd	54446	9.9273	-7471B		PPB	11 Jul 2019 14:34:02	U	SMPL
ChkStd - 1	ChkStd	38081	6.9419	-7471B		PPB	11 Jul 2019 14:36:18	U	SMPL
PB121303BL - 1	PBS	-59	-0.0158	-7471B		PPB	11 Jul 2019 14:38:36	U	SMPL
PB121303BS - 1	LCSS	20539	3.7418	-7471B		PPB	11 Jul 2019 14:40:54	U	SMPL
K3621-01 - 1	OK-03-071019-A	1200	0.2138	-7471B		PPB	11 Jul 2019 14:43:11	U	SMPL
K3621-01DUP - 1	OK-03-071019-ADUP	1061	0.1885	-7471B		PPB	11 Jul 2019 14:45:28	U	SMPL
K3621-01MS - 1	OK-03-071019-AMS	21935	3.9964	-7471B		PPB	11 Jul 2019 14:47:46	U	SMPL
K3621-01MSD - 1	OK-03-071019-AMSD	22097	4.0260	-7471B		PPB	11 Jul 2019 14:50:03	U	SMPL
K3621-03 - 1	OK-03-071019-B	836	0.1474	-7471B		PPB	11 Jul 2019 14:52:19	U	SMPL
CCV17 - 1	CCV17	27698	5.0478	-7471B		PPB	11 Jul 2019 14:54:36	U	SMPL
CCB17 - 1	CCB17	-41	-0.0126	-7471B		PPB	11 Jul 2019 14:56:53	U	SMPL
K3726-06 - 1	COMP-1_070919	459	0.0787	-7471B		PPB	11 Jul 2019 14:59:10	U	SMPL
K3751-01 - 1	MANHOLE-TEST-PIT	795	0.1399	-7471B		PPB	11 Jul 2019 15:01:28	U	SMPL
K3751-03 - 1	DUCT-BANK-TEST-PIT	220	0.0351	-7471B		PPB	11 Jul 2019 15:03:44	U	SMPL
K3621-01LX5 - 1		217	0.0345	-7471B		PPB	11 Jul 2019 15:06:00	U	SMPL
K3621-01A - 1		21938	3.9970	-7471B		PPB	11 Jul 2019 15:08:17	U	SMPL
CCV18 - 1	CCV18	27302	4.9755	-7471B		PPB	11 Jul 2019 15:10:34	U	SMPL
CCB18 - 1	CCB18	0	-0.0051	-7471B		PPB	11 Jul 2019 15:12:52	U	SMPL