

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

7/11/2019 15:05

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.007	0.0	0.121	
ICB1	0.005	0.0	0.012	
CCV1	1.013	0.0	0.122	
CCB1	0.003	0.0	0.012	
PB121275BL	0.003	0.0	0.012	
PB12175BS	1.016	0.0	0.123	
K3591-10	0.008	0.0	0.012	
K3591-11	0.049	0.0	0.017	
CCV2	1.007	0.0	0.122	
CCB3	0.001	0.0	0.011	

N	10
Mean	0.411
SD	0.5162
CV%	125.58

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

Instrument ID : Konelab

7/11/2019 13:53


Test Phenolics-

Accepted 7/11/2019 13:53

Factor 9.136
Bias 0.011

Coeff. of det. 0.999958

Errors

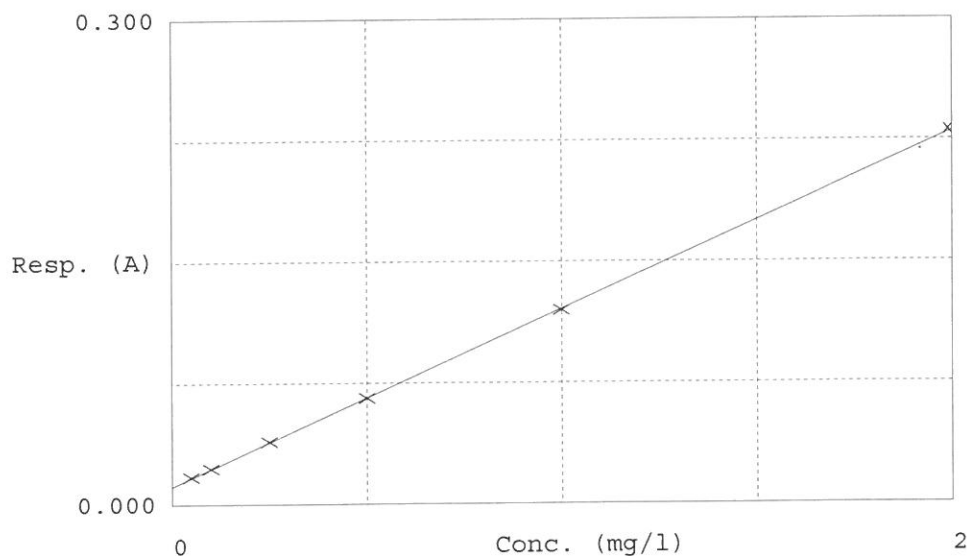

	Calibrator	Response	Calc. con.	Conc.	Errors <i>percentage %</i>
1	Phenol-2	0.017	0.0538	0.0500	108 %
2	Phenol-2	0.022	0.1008	0.1000	101 %
3	Phenol-2	0.039	0.2523	0.2500	101 %
4	Phenol-2	0.066	0.4968	0.5000	99 %
5	Phenol-2	0.120	0.9918	1.0000	99 %
6	Phenol-2	0.231	2.0045	2.0000	100 %

AS
07/11/19

Aquakem v. 7.2AQ1

Results from time period:

Thu Jul 11 15:05:15 2019

Thu Jul 11 15:05:24 2019

AS

Sample Id	Sam/Ctr/c/	Test short na	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0538	mg/l	7/11/2019 13:42:46	
0.1PPM	A	Phenolics-	P	0.1008	mg/l	7/11/2019 13:42:47	
0.25PPM	A	Phenolics-	P	0.2523	mg/l	7/11/2019 13:42:48	
0.50PPM	A	Phenolics-	P	0.4968	mg/l	7/11/2019 13:42:49	
1.0PPM	A	Phenolics-	P	0.9918	mg/l	7/11/2019 13:42:50	
2.0PPM	A	Phenolics-	P	2.0045	mg/l	7/11/2019 13:42:51	
ICV1	S	Phenolics-	P	1.0068	mg/l	7/11/2019 15:05:15	
ICB1	S	Phenolics-	P	0.0046	mg/l	7/11/2019 15:05:16	
CCV1	S	Phenolics-	P	1.0126	mg/l	7/11/2019 15:05:17	
CCB1	S	Phenolics-	P	0.0033	mg/l	7/11/2019 15:05:18	
PB121275BL	S	Phenolics-	P	0.003	mg/l	7/11/2019 15:05:19	
PB12175BS	S	Phenolics-	P	1.0161	mg/l	7/11/2019 15:05:20	
K3591-10	S	Phenolics-	P	0.0075	mg/l	7/11/2019 15:05:21	
K3591-11	S	Phenolics-	P	0.0487	mg/l	7/11/2019 15:05:22	
CCV2	S	Phenolics-	P	1.0072	mg/l	7/11/2019 15:05:23	
CCB3	S	Phenolics-	P	0.001	mg/l	7/11/2019 15:05:24	