


LB103925

7470A

INSTRUMENT ID : CUI

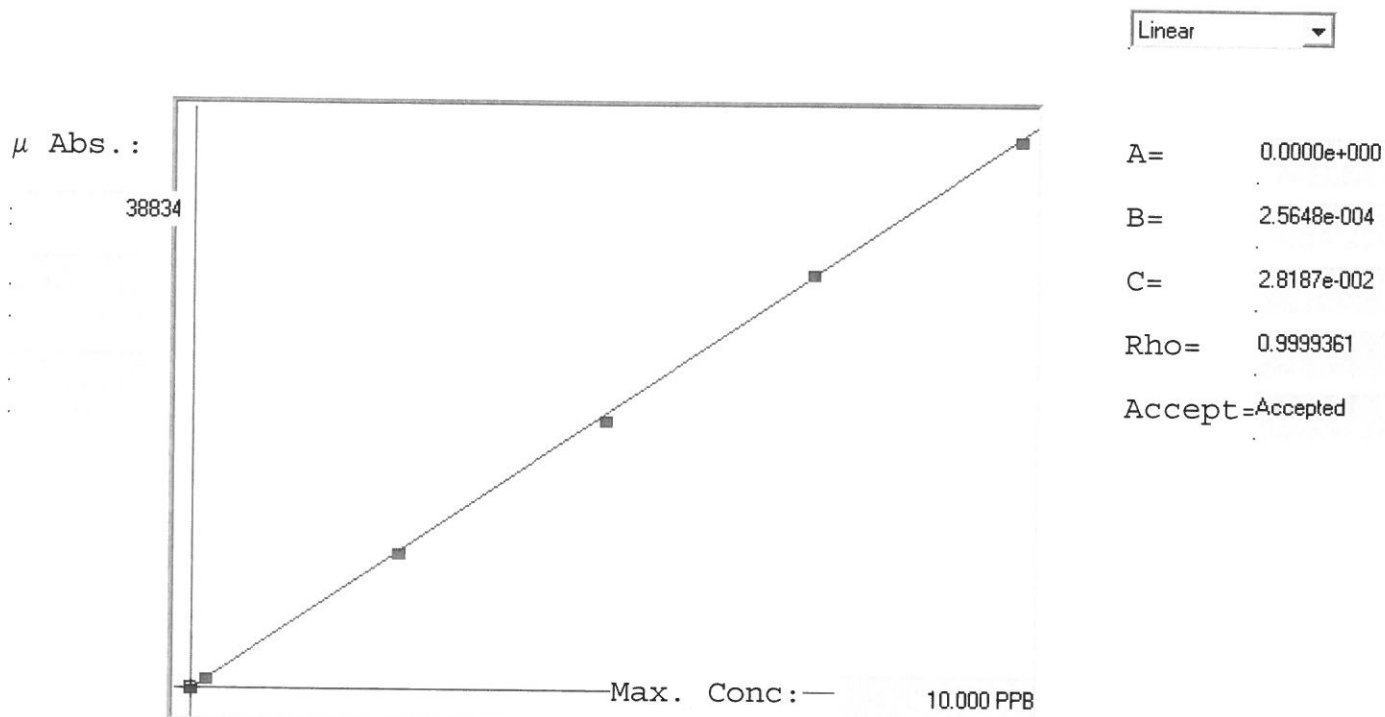

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.022	0.022	-24	0.000	-24				
0.2	0.200	0.202	0.002	677	0.0 %	677				
2.5	2.500	2.498	-0.002	9630	0.0 %	9630				
5.0	5.000	4.925	-0.075	19092	0.0 %	19092				
7.5	7.500	7.565	0.065	29384	0.0 %	29384				
10.0	10.000	9.988	-0.012	38834	0.0 %	38834				

LB103925 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 12 Jul 2019 10:51:38

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50-0	-24	-	0.00007470A	PPB	12 Jul 2019 11:03:48	S	Std
0.2 - 1	50-2	677	-	0.20007470A	PPB	12 Jul 2019 11:06:17	S	Std
2.5 - 1	52-5	9630	-	2.50007470A	PPB	12 Jul 2019 11:08:25	S	Std
5.0 - 1	55-0	19092	-	5.00007470A	PPB	12 Jul 2019 11:10:33	S	Std
7.5 - 1	57-5	29384	-	7.50007470A	PPB	12 Jul 2019 11:12:41	S	Std
10.0 - 1	510-0	38834	-	10.00007470A	PPB	12 Jul 2019 11:14:48	S	Std
ICV31 - 1	ICV31	15567	4.0208	-7470A	PPB	12 Jul 2019 11:17:19	U	SMPL
ICB31 - 1	ICB31	68	0.0456	-7470A	PPB	12 Jul 2019 11:19:26	U	SMPL
CCV19 - 1	CCV19	19103	4.9278	-7470A	PPB	12 Jul 2019 11:21:32	U	SMPL
CCB19 - 1	CCB19	-68	0.0107	-7470A	PPB	12 Jul 2019 11:23:38	U	SMPL
CRA - 1	CRA	667	0.1993	-7470A	PPB	12 Jul 2019 11:25:45	U	SMPL
HighStd - 1	HighStd	38702	9.9546	-7470A	PPB	12 Jul 2019 11:27:51	U	SMPL
ChkStd - 1	ChkStd	26720	6.8814	-7470A	PPB	12 Jul 2019 11:29:58	U	SMPL
PB121338BL - 1	PBW	-73	0.0095	-7470A	PPB	12 Jul 2019 11:32:06	U	SMPL
PB121338BS - 1	LCSW	15903	4.1070	-7470A	PPB	12 Jul 2019 11:34:13	U	SMPL
K3621-02 - 1	OK-03-071019-A	-4	0.0272	-7470A	PPB	12 Jul 2019 11:36:20	U	SMPL
K3621-02DUP - 1	OK-03-071019-ADUP	67	0.0454	-7470A	PPB	12 Jul 2019 11:38:28	U	SMPL
K3621-02MS - 1	OK-03-071019-AMS	16935	4.3717	-7470A	PPB	12 Jul 2019 11:40:36	U	SMPL
K3621-02MSD - 1	OK-03-071019-AMSD	15144	3.9124	-7470A	PPB	12 Jul 2019 11:42:45	U	SMPL
K3621-04 - 1	OK-03-071019-B	-13	0.0249	-7470A	PPB	12 Jul 2019 11:44:51	U	SMPL
CCV20 - 1	CCV20	19306	4.9798	-7470A	PPB	12 Jul 2019 11:46:58	U	SMPL
CCB20 - 1	CCB20	-44	0.0169	-7470A	PPB	12 Jul 2019 11:49:05	U	SMPL
K3735-01 - 1	1586	457	0.1454	-7470A	PPB	12 Jul 2019 11:51:12	U	SMPL
K3740-07 - 1	COMP-22	-150	-0.0103	-7470A	PPB	12 Jul 2019 11:53:19	U	SMPL
K3740-08 - 1	COMP-23	-20	0.0231	-7470A	PPB	12 Jul 2019 11:55:26	U	SMPL
K3740-09 - 1	COMP-24	-4	0.0272	-7470A	PPB	12 Jul 2019 11:57:32	U	SMPL
PB121339BL - 1	PBW	-4	0.0272	-7470A	PPB	12 Jul 2019 11:59:39	U	SMPL
PB121339BS - 1	LCSW	15735	4.0639	-7470A	PPB	12 Jul 2019 12:01:47	U	SMPL
K3641-02 - 1	FM-5210	-26	0.0215	-7470A	PPB	12 Jul 2019 12:03:54	U	SMPL
K3641-02DUP - 1	FM-5210DUP	21	0.0336	-7470A	PPB	12 Jul 2019 12:06:02	U	SMPL
K3641-02MS - 1	FM-5210MS	16007	4.1337	-7470A	PPB	12 Jul 2019 12:08:10	U	SMPL
K3641-02MSD - 1	FM-5210MSD	15550	4.0165	-7470A	PPB	12 Jul 2019 12:10:17	U	SMPL
CCV21 - 1	CCV21	19100	4.9270	-7470A	PPB	12 Jul 2019 12:12:24	U	SMPL
CCB21 - 1	CCB21	-29	0.0207	-7470A	PPB	12 Jul 2019 12:14:31	U	SMPL
PB121340BL - 1	PBW	-8	0.0261	-7470A	PPB	12 Jul 2019 12:16:37	U	SMPL
PB121340BS - 1	LCSW	15946	4.1181	-7470A	PPB	12 Jul 2019 12:18:44	U	SMPL
K3618-04 - 1	HD-02-071119	-7	0.0264	-7470A	PPB	12 Jul 2019 12:20:51	U	SMPL
K3618-04DUP - 1	HD-02-071119DUP	19	0.0331	-7470A	PPB	12 Jul 2019 12:22:58	U	SMPL
K3618-04MS - 1	HD-02-071119MS	14556	3.7615	-7470A	PPB	12 Jul 2019 12:25:05	U	SMPL
K3618-04MSD - 1	HD-02-071119MSD	14591	3.7705	-7470A	PPB	12 Jul 2019 12:27:12	U	SMPL
K3626-06 - 1	SU-04-071119-A	-24	0.0220	-7470A	PPB	12 Jul 2019 12:29:20	U	SMPL
K3626-08 - 1	SU-04-071119-B	1	0.0284	-7470A	PPB	12 Jul 2019 12:31:28	U	SMPL
K3761-02 - 1	SOIL-DRUM	22	0.0338	-7470A	PPB	12 Jul 2019 12:33:37	U	SMPL
K3768-33 - 1	SOIL-COMP	20	0.0333	-7470A	PPB	12 Jul 2019 12:35:44	U	SMPL
CCV22 - 1	CCV22	18204	4.6972	-7470A	PPB	12 Jul 2019 12:41:21	U	SMPL
CCB22 - 1	CCB22	-23	0.0223	-7470A	PPB	12 Jul 2019 12:43:27	U	SMPL
K3775-02 - 1	D-3-ROLL-OFF-DUMPSTER-3	-1	0.0279	-7470A	PPB	12 Jul 2019 12:45:34	U	SMPL
PB121338TB - 1	PB121282TB	11	0.0310	-7470A	PPB	12 Jul 2019 12:47:40	U	SMPL
PB121339TB - 1	PB121267TB	1	0.0284	-7470A	PPB	12 Jul 2019 12:49:47	U	SMPL
PB121340TB - 1	PB121317TB	15	0.0320	-7470A	PPB	12 Jul 2019 12:51:54	U	SMPL
K3621-02LX5 - 1		-4	0.0272	-7470A	PPB	12 Jul 2019 12:54:01	U	SMPL
K3621-02A - 1		15093	3.8993	-7470A	PPB	12 Jul 2019 12:56:09	U	SMPL
K3641-02LX5 - 1		-36	0.0190	-7470A	PPB	12 Jul 2019 12:58:17	U	SMPL
K3641-02A - 1		15121	3.9065	-7470A	PPB	12 Jul 2019 13:00:25	U	SMPL
K3618-04LX5 - 1		-11	0.0254	-7470A	PPB	12 Jul 2019 13:02:34	U	SMPL
K3618-04A - 1		14461	3.7372	-7470A	PPB	12 Jul 2019 13:04:41	U	SMPL
CCV23 - 1	CCV23	18353	4.7354	-7470A	PPB	12 Jul 2019 13:06:47	U	SMPL
CCB23 - 1	CCB23	-4	0.0272	-7470A	PPB	12 Jul 2019 13:08:55	U	SMPL