

Lb104020

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : CT

Instrument ID : Konelab

7/17/2019 12:13


Test Total CN

Accepted 7/17/2019 12:13

Factor 1057
 Bias 0.002

Coeff. of det. 0.999905

Errors

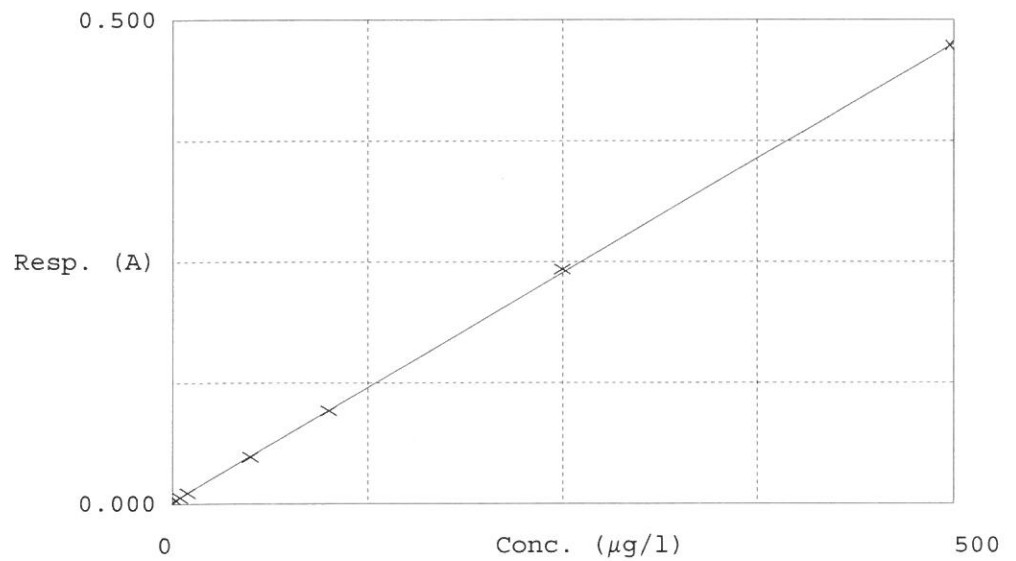

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.3360	0.0000	
2	5.0PPBCN	0.007	4.7967	5.0000	
3	10PPBCN	0.011	9.7979	10.0000	
4	50PPBCN	0.049	49.0883	50.0000	
5	100PPBCN	0.096	99.5142	100.0000	
6	250PPBCN	0.242	253.8890	250.0000	
7	500PPBCN	0.474	498.2499	500.0000	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

7/17/2019 15:26

Sample id	Test id	Result	Status	Date	Errors
ICV1	Total CN	98.288	man acc	7/17/2019	
ICB1	Total CN	0.523	man acc	7/17/2019	
CCV1	Total CN	247.940	man acc	7/17/2019	
CCB1	Total CN	0.647	man acc	7/17/2019	
PB121452BL	Total CN	0.742	man acc	7/17/2019	
PB121452BS	Total CN	98.760	man acc	7/17/2019	
MIDPB121452	Total CN	249.629	man acc	7/17/2019	
K3853-01	Total CN	56.853	man acc	7/17/2019	
K3853-01DUP	Total CN	57.108	man acc	7/17/2019	
K3853-01MS	Total CN	96.761	man acc	7/17/2019	
K3853-01MSD	Total CN	98.218	man acc	7/17/2019	
CCV2	Total CN	258.617	man acc	7/17/2019	
CCB2	Total CN	0.459	man acc	7/17/2019	

CT

Aquakem v. 7.2AQ1

Results from time period:

Wed Jul 17 10:38:41 2019

Wed Jul 17 13:19:04 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result uni	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.336	µg/l	7/17/2019 10:38:41	
5.0PPBCN	A	Total CN	P	4.7967	µg/l	7/17/2019 10:38:42	
10PPBCN	A	Total CN	P	9.7979	µg/l	7/17/2019 10:38:43	
50PPBCN	A	Total CN	P	49.0883	µg/l	7/17/2019 10:38:44	
100PPBCN	A	Total CN	P	99.5142	µg/l	7/17/2019 10:38:45	
250PPBCN	A	Total CN	P	253.889	µg/l	7/17/2019 10:38:46	
500PPBCN	A	Total CN	P	498.2499	µg/l	7/17/2019 10:38:47	
ICV1	S	Total CN	P	98.288	µg/l	7/17/2019 13:14:13	
ICB1	S	Total CN	P	0.5225	µg/l	7/17/2019 13:14:14	
CCV1	S	Total CN	P	247.9399	µg/l	7/17/2019 13:14:15	
CCB1	S	Total CN	P	0.6472	µg/l	7/17/2019 13:14:16	
PB121452BL	S	Total CN	P	0.7419	µg/l	7/17/2019 13:14:17	
PB121452BS	S	Total CN	P	98.7599	µg/l	7/17/2019 13:14:18	
MIDPB121452	S	Total CN	P	249.6285	µg/l	7/17/2019 13:14:19	
K3853-01	S	Total CN	P	56.8533	µg/l	7/17/2019 13:14:20	
K3853-01DUP	S	Total CN	P	57.1079	µg/l	7/17/2019 13:14:21	
K3853-01MS	S	Total CN	P	96.7611	µg/l	7/17/2019 13:14:22	
K3853-01MSD	S	Total CN	P	98.2177	µg/l	7/17/2019 13:19:00	
CCV2	S	Total CN	P	258.6175	µg/l	7/17/2019 13:19:02	
CCB2	S	Total CN	P	0.4586	µg/l	7/17/2019 13:19:03	