

LB104048


7470A

INSTRUMENT ID : CV1

Linear

 μ Abs. :

39178

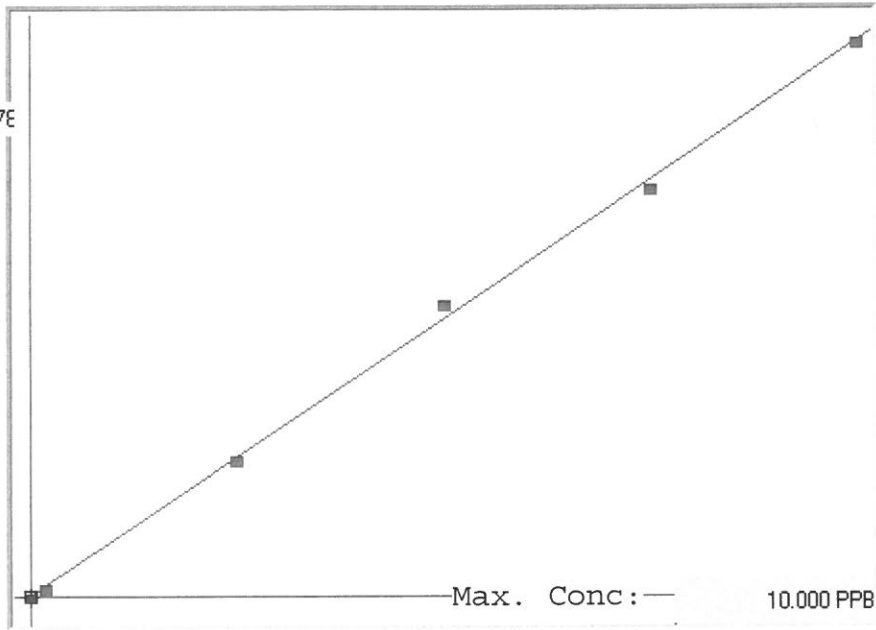

A= 0.0000e+000

B= 2.5504e-004

C= -6.2996e-003

Rho= 0.9994161

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.025	-0.025	-75	0.000	-75				
0.2	0.200	0.166	-0.034	674	0.0 %	674				
2.5	2.500	2.470	-0.030	9709	0.0 %	9709				
5.0	5.000	5.261	0.261	20652	0.0 %	20652				
7.5	7.500	7.344	-0.156	28819	0.0 %	28819				
10.0	10.000	9.986	-0.014	39178	0.0 %	39178				

LB104048 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 17 Jul 2019 10:07:50				
Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type
0.0 - 1	00-0	26	-	0.00007470A	PPB		17 Jul 2019 10:11:48	S Std
0.2 - 1	50-2	834	-	0.20007470A	PPB		17 Jul 2019 10:13:57	S Std
2.5 - 1	52-5	10441	-	2.50007470A	PPB		17 Jul 2019 10:16:06	S Std
5.0 - 1	55-0	19674	-	5.00007470A	PPB		17 Jul 2019 10:18:14	S Std
7.5 - 1	57-5	28871	-	7.50007470A	PPB		17 Jul 2019 10:20:23	S Std
10.0 - 1	510-0	40155	-	10.00007470A	PPB		17 Jul 2019 10:27:30	S Std
ICV35 - 1	ICV35	15178	3.8235	-7470A	PPB		17 Jul 2019 10:30:05	U SMPL
ICB35 - 1	ICB35	-10	-0.0177	-7470A	PPB		17 Jul 2019 10:32:11	U SMPL
CCV36 - 1	CCV36	19887	5.0144	-7470A	PPB		17 Jul 2019 10:34:18	U SMPL
CCB36 - 1	CCB36	103	0.0109	-7470A	PPB		17 Jul 2019 10:36:25	U SMPL
CRA - 1	CRA	833	0.1955	-7470A	PPB		17 Jul 2019 10:38:31	U SMPL
HighStd - 1	HighStd	41081	10.3745	-7470A	PPB		17 Jul 2019 10:40:42	U SMPL
ChkStd - 1	ChkStd	28681	7.2385	-7470A	PPB		17 Jul 2019 10:42:49	U SMPL
PB121449BL - 1	PBW	-51	-0.0280	-7470A	PPB		17 Jul 2019 10:44:57	U SMPL
PB121449BS - 1	LCSW	16249	4.0943	-7470A	PPB		17 Jul 2019 10:47:04	U SMPL
K3620-02 - 1	CL-01-071219-A	-13	-0.0184	-7470A	PPB		17 Jul 2019 10:49:12	U SMPL
K3620-02DUP - 1	CL-01-071219-ADUP	23	-0.0093	-7470A	PPB		17 Jul 2019 10:51:20	U SMPL
K3620-02MS - 1	CL-01-071219-AMS	16151	4.0695	-7470A	PPB		17 Jul 2019 10:53:28	U SMPL
K3620-02MSD - 1	CL-01-071219-AMSD	16146	4.0683	-7470A	PPB		17 Jul 2019 10:55:36	U SMPL
K3620-04 - 1	CL-01-071219-B	-24	-0.0212	-7470A	PPB		17 Jul 2019 10:57:44	U SMPL
CCV37 - 1	CCV37	19770	4.9848	-7470A	PPB		17 Jul 2019 10:59:52	U SMPL
CCB37 - 1	CCB37	-17	-0.0194	-7470A	PPB		17 Jul 2019 11:01:58	U SMPL
K3620-06 - 1	CL-01-071219-C	9	-0.0129	-7470A	PPB		17 Jul 2019 11:04:05	U SMPL
K3620-08 - 1	CL-01-071219-D	10	-0.0126	-7470A	PPB		17 Jul 2019 11:06:12	U SMPL
K3620-10 - 1	CL-01-071219-E	20	-0.0101	-7470A	PPB		17 Jul 2019 11:08:18	U SMPL
PB121450BL - 1	PBW	16	-0.0111	-7470A	PPB		17 Jul 2019 11:10:25	U SMPL
PB121450BS - 1	LCSW	16306	4.1087	-7470A	PPB		17 Jul 2019 11:12:32	U SMPL
K3622-06 - 1	OR-03-071519-A	-7	-0.0169	-7470A	PPB		17 Jul 2019 11:14:40	U SMPL
K3622-06DUP - 1	OR-03-071519-ADUP	14	-0.0116	-7470A	PPB		17 Jul 2019 11:16:47	U SMPL
K3622-06MS - 1	OR-03-071519-AMS	16354	4.1209	-7470A	PPB		17 Jul 2019 11:18:55	U SMPL
K3622-06MSD - 1	OR-03-071519-AMSD	15937	4.0154	-7470A	PPB		17 Jul 2019 11:21:04	U SMPL
K3622-08 - 1	OR-03-071519-B	-5	-0.0164	-7470A	PPB		17 Jul 2019 11:23:10	U SMPL
CCV38 - 1	CCV38	19493	4.9148	-7470A	PPB		17 Jul 2019 11:25:17	U SMPL
CCB38 - 1	CCB38	-31	-0.0230	-7470A	PPB		17 Jul 2019 11:27:23	U SMPL
K3623-02 - 1	EO-02-071519-A	7	-0.0134	-7470A	PPB		17 Jul 2019 11:29:31	U SMPL
K3623-04 - 1	EO-02-071519-B	18	-0.0106	-7470A	PPB		17 Jul 2019 11:31:37	U SMPL
K3623-06 - 1	EO-02-071519-C	20	-0.0101	-7470A	PPB		17 Jul 2019 11:33:44	U SMPL
K3627-04 - 1	TR-04-071519	14	-0.0116	-7470A	PPB		17 Jul 2019 11:35:51	U SMPL
K3820-02 - 1	RBR-200050	4	-0.0141	-7470A	PPB		17 Jul 2019 11:37:58	U SMPL
K3826-02 - 1	RBR-200034	21	-0.0098	-7470A	PPB		17 Jul 2019 11:40:06	U SMPL
K3826-04 - 1	RBR-200036	16	-0.0111	-7470A	PPB		17 Jul 2019 11:42:15	U SMPL
K3829-01 - 1	IDW-EW03-TRENCH	142	0.0208	-7470A	PPB		17 Jul 2019 11:44:32	U SMPL
K3829-02 - 1	IDW-EW03-CONCRETE	-6	-0.0167	-7470A	PPB		17 Jul 2019 11:46:41	U SMPL
K3830-02 - 1	RT-3456	8	-0.0131	-7470A	PPB		17 Jul 2019 11:48:48	U SMPL
CCV39 - 1	CCV39	19762	4.9828	-7470A	PPB		17 Jul 2019 11:53:36	U SMPL
CCB39 - 1	CCB39	-8	-0.0172	-7470A	PPB		17 Jul 2019 11:55:43	U SMPL
K3830-04 - 1	RT-4651	6	-0.0136	-7470A	PPB		17 Jul 2019 11:57:50	U SMPL
K3830-06 - 1	RT-1873	24	-0.0091	-7470A	PPB		17 Jul 2019 11:59:56	U SMPL
K3830-08 - 1	RBR-200027	17	-0.0108	-7470A	PPB		17 Jul 2019 12:02:04	U SMPL
PB121449TB - 1	PB121353TB	31	-0.0073	-7470A	PPB		17 Jul 2019 12:04:11	U SMPL
PB121450TB - 1	PB121397TB	28	-0.0081	-7470A	PPB		17 Jul 2019 12:06:18	U SMPL
K3620-02LX5 - 1		4	-0.0141	-7470A	PPB		17 Jul 2019 12:08:26	U SMPL
K3620-02A - 1		16285	4.1034	-7470A	PPB		17 Jul 2019 12:10:34	U SMPL
K3622-06LX5 - 1		-9	-0.0174	-7470A	PPB		17 Jul 2019 12:12:42	U SMPL
K3622-06A - 1		16257	4.0964	-7470A	PPB		17 Jul 2019 12:14:51	U SMPL
CCV40 - 1	CCV40	20314	5.1224	-7470A	PPB		17 Jul 2019 12:16:59	U SMPL
CCB40 - 1	CCB40	-33	-0.0235	-7470A	PPB		17 Jul 2019 12:19:07	U SMPL
0.0 - 1		-75	-	0.00007470A	PPB		18 Jul 2019 10:59:00	S Std
0.2 - 1		674	-	0.20007470A	PPB		18 Jul 2019 11:01:10	S Std
2.5 - 1		9709	-	2.50007470A	PPB		18 Jul 2019 11:03:19	S Std
5.0 - 1		20652	-	5.00007470A	PPB		18 Jul 2019 11:05:27	S Std
7.5 - 1		28819	-	7.50007470A	PPB		18 Jul 2019 11:07:36	S Std
10.0 - 1		39178	-	10.00007470A	PPB		18 Jul 2019 11:09:43	S Std
ICV36 - 1	ICV36	15462	3.9371	-7470A	PPB		18 Jul 2019 11:12:46	U SMPL
ICB36 - 1	ICB36	-56	-0.0206	-7470A	PPB		18 Jul 2019 11:14:53	U SMPL
CCV41 - 1	CCV41	20659	5.2625	-7470A	PPB		18 Jul 2019 11:16:59	U SMPL
CCB41 - 1	CCB41	-64	-0.0226	-7470A	PPB		18 Jul 2019 11:19:05	U SMPL
CRA - 1	CRA	699	0.1720	-7470A	PPB		18 Jul 2019 11:21:12	U SMPL
HighStd - 1	HighStd	39798	10.1437	-7470A	PPB		18 Jul 2019 11:23:18	U SMPL
ChkStd - 1	ChkStd	27302	6.9567	-7470A	PPB		18 Jul 2019 11:25:25	U SMPL
PB121488BL - 1	PBW	-75	-0.0254	-7470A	PPB		18 Jul 2019 11:27:32	U SMPL
PB121488BS - 1	LCSW	15966	4.0656	-7470A	PPB		18 Jul 2019 11:29:40	U SMPL
K3836-01 - 1	JOYCE-SW-7-12	22	-0.0007	-7470A	PPB		18 Jul 2019 11:31:47	U SMPL
K3836-01DUP - 1	JOYCE-SW-7-12DUP	50	0.0065	-7470A	PPB		18 Jul 2019 11:33:55	U SMPL
K3836-01MS - 1	JOYCE-SW-7-12MS	15540	3.9570	-7470A	PPB		18 Jul 2019 11:36:03	U SMPL
K3836-01MSD - 1	JOYCE-SW-7-12MSD	15624	3.9784	-7470A	PPB		18 Jul 2019 11:38:12	U SMPL
K3838-03 - 1	WARINANCO-CITY-SEWER-INSTALL	14609	3.7196	-7470A	PPB		18 Jul 2019 11:40:18	U SMPL
CCV42 - 1	CCV42	20228	5.1526	-7470A	PPB		18 Jul 2019 11:42:25	U SMPL
CCB42 - 1	CCB42	-66	-0.0231	-7470A	PPB		18 Jul 2019 11:44:33	U SMPL
K3836-01LX5 - 1		-7	-0.0081	-7470A	PPB		18 Jul 2019 11:46:39	U SMPL
K3836-01A - 1		15244	3.8815	-7470A	PPB		18 Jul 2019 11:48:46	U SMPL
CCV43 - 1	CCV43	19972	5.0873	-7470A	PPB		18 Jul 2019 11:50:53	U SMPL
CCB43 - 1	CCB43	-51	-0.0193	-7470A	PPB		18 Jul 2019 11:53:00	U SMPL