


LB104075

245.1

INSTRUMENT ID : CV1

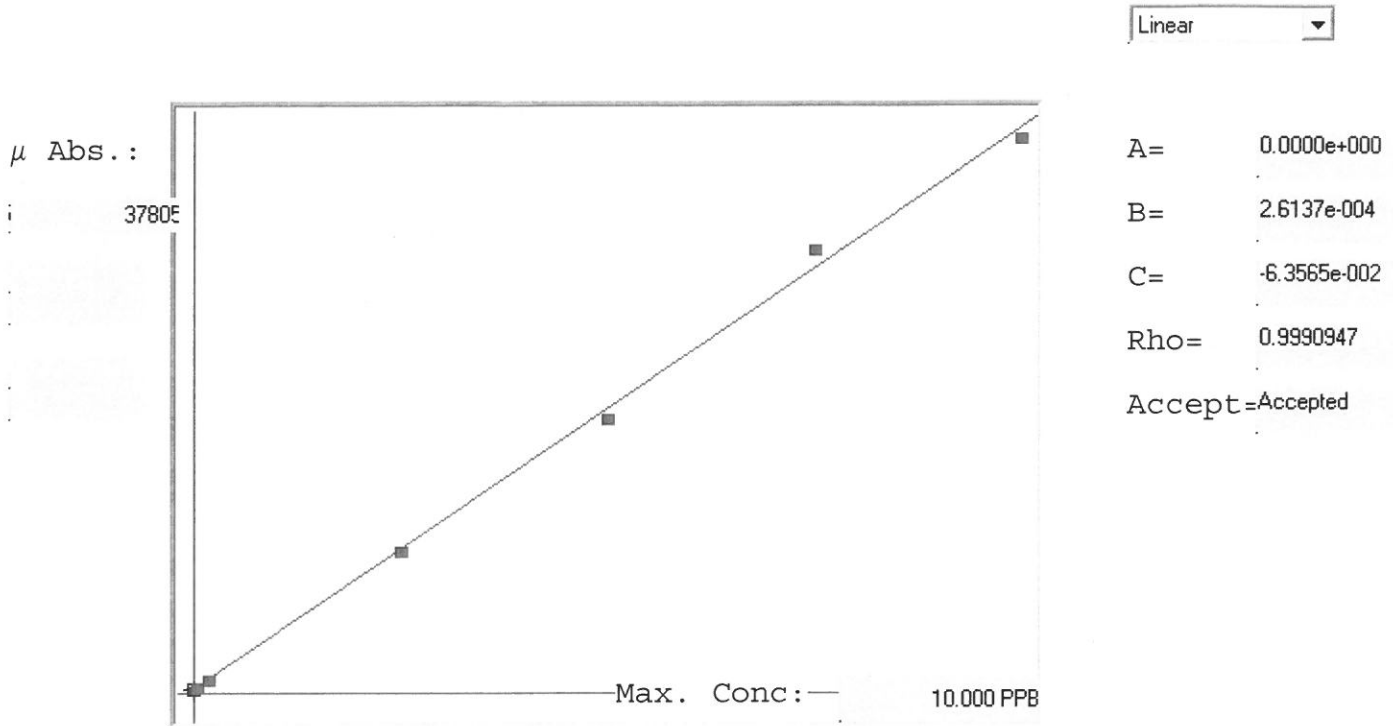

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.020	0.020	321	0.000	321				
0.05	0.050	0.063	0.013	486	0.0 %	486				
0.2	0.200	0.200	0.000	1009	0.0 %	1009				
2.5	2.500	2.474	-0.026	9709	0.0 %	9709				
5.0	5.000	4.838	-0.162	18752	0.0 %	18752				
7.5	7.500	7.837	0.337	30228	0.0 %	30228				
10.0	10.000	9.817	-0.183	37805	0.0 %	37805				

LB104075 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 19 Jul 2019 09:08:00

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50-0	321	-	0.000245.1	PPB	19 Jul 2019 09:09:55	S	Std
0.05 - 1	50-65	486	-	0.0500245.1	PPB	19 Jul 2019 09:12:13	S	Std
0.2 - 1	50-2	1009	-	0.2000245.1	PPB	19 Jul 2019 09:14:31	S	Std
2.5 - 1	52-5	9709	-	2.5000245.1	PPB	19 Jul 2019 09:16:50	S	Std
5.0 - 1	55-0	18752	-	5.0000245.1	PPB	19 Jul 2019 09:19:07	S	Std
7.5 - 1	57-5	30228	-	7.5000245.1	PPB	19 Jul 2019 09:21:23	S	Std
10.0 - 1	57-0	37805	-	10.0000245.1	PPB	19 Jul 2019 09:23:40	S	Std
ICV39 - 1	ICV39	14784	3.8005	-245.1	PPB	19 Jul 2019 09:32:05	U	SMPL
ICB39 - 1	ICB39	305	0.0162	-245.1	PPB	19 Jul 2019 09:34:20	U	SMPL
CCV53 - 1	CCV53	18703	4.8248	-245.1	PPB	19 Jul 2019 09:36:35	U	SMPL
CCB53 - 1	CCB53	338	0.0248	-245.1	PPB	19 Jul 2019 09:38:52	U	SMPL
CRA - 1	CRA	398	0.0405	-245.1	PPB	19 Jul 2019 10:19:06	U	SMPL
HighStd - 1	HighStd	38422	9.9787	-245.1	PPB	19 Jul 2019 10:21:21	U	SMPL
ChkStd - 1	ChkStd	27473	7.1170	-245.1	PPB	19 Jul 2019 10:23:38	U	SMPL
PB121531BL - 1	PBW	170	-0.0191	-245.1	PPB	19 Jul 2019 10:29:37	U	SMPL
PB121531BS - 1	LCSW	17726	4.5694	-245.1	PPB	19 Jul 2019 10:31:53	U	SMPL
K3744-01 - 1	EFF-DAY-1-METALS	837	0.1552	-245.1	PPB	19 Jul 2019 10:34:11	U	SMPL
K3905-01 - 1	18107-NYCT-AVE-Z-TWP-1	38986	10.1261	-245.1	PPB	19 Jul 2019 10:51:57	U	SMPL
K3905-01DUP - 1	18107-NYCT-AVE-Z-TWP-1DUP	38242	9.9316	-245.1	PPB	19 Jul 2019 10:54:14	U	SMPL
K3905-01MS - 1	18107-NYCT-AVE-Z-TWP-1MS	63641	16.5701	-245.1	PPB	19 Jul 2019 10:56:33	U	SMPL
K3905-01MSD - 1	18107-NYCT-AVE-Z-TWP-1MSD	64957	16.9140	-245.1	PPB	19 Jul 2019 10:58:51	U	SMPL
CCV54 - 1	CCV54	18477	4.7657	-245.1	PPB	19 Jul 2019 11:01:09	U	SMPL
CCB54 - 1	CCB54	76	-0.0437	-245.1	PPB	19 Jul 2019 11:03:27	U	SMPL
K3905-01LX5 - 1		7882	1.9965	-245.1	PPB	19 Jul 2019 11:05:43	U	SMPL
K3905-01A - 1		65074	16.9446	-245.1	PPB	19 Jul 2019 11:07:59	U	SMPL
K3905-01DLX3 - 1		12472	3.1962	-245.1	PPB	19 Jul 2019 11:21:44	U	SMPL
K3905-01DUPDLX3 - 1		12760	3.2715	-245.1	PPB	19 Jul 2019 11:24:00	U	SMPL
K3905-01MSDLX3 - 1		20074	5.1831	-245.1	PPB	19 Jul 2019 11:26:16	U	SMPL
K3905-01MSDDLX3 - 1		20671	5.3391	-245.1	PPB	19 Jul 2019 11:28:33	U	SMPL
K3905-01DLX15 - 1		2270	0.5297	-245.1	PPB	19 Jul 2019 11:30:50	U	SMPL
K3905-01ADLX3 - 1		21530	5.5637	-245.1	PPB	19 Jul 2019 11:33:08	U	SMPL
CCV55 - 1	CCV55	18861	4.8661	-245.1	PPB	19 Jul 2019 11:35:25	U	SMPL
CCB55 - 1	CCB55	748	0.1319	-245.1	PPB	19 Jul 2019 11:37:41	U	SMPL