

LB104100

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

7/19/2019 14:44

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.014	0.0	0.122	
ICB1	0.004	0.0	0.012	
CCV1	1.001	0.0	0.121	
CCB1	0.002	0.0	0.012	
PB121520BL	0.002	0.0	0.012	
PB121520BS	1.022	0.0	0.123	
K3834-15	0.005	0.0	0.012	
K3834-15DUP	0.003	0.0	0.012	
K3834-15MS	0.967	0.0	0.117	
K3834-15MSD	0.969	0.0	0.117	
K3882-01	0.001	0.0	0.012	
K3883-01	0.001	0.0	0.012	
K3905-01	0.002	0.0	0.012	
K3908-01	0.031	0.0	0.015	
CCV2	0.999	0.0	0.121	
CCB2	-0.004	0.0	0.011	

N	16
Mean	0.376
SD	0.4956
CV%	131.71

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

7/19/2019 14:05


Test Phenolics-

Accepted 7/19/2019 14:05

Factor 9.148
Bias 0.012

Coeff. of det. 0.999986

Errors

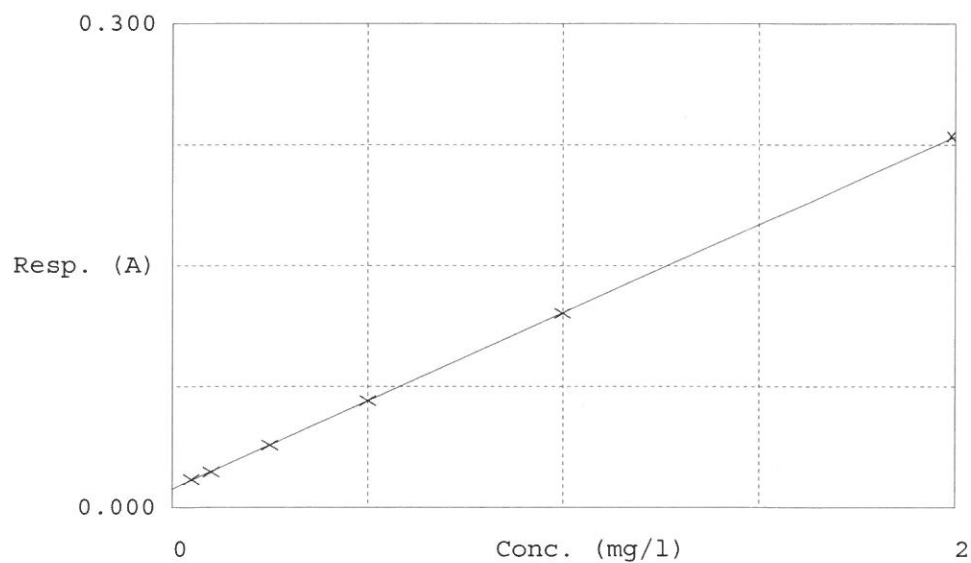

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.017	0.0542	0.0500	
2	Phenol-2	0.022	0.0968	0.1000	
3	Phenol-2	0.039	0.2497	0.2500	
4	Phenol-2	0.066	0.5009	0.5000	
5	Phenol-2	0.120	0.9971	1.0000	
6	Phenol-2	0.230	2.0013	2.0000	

CT

Aquakem v. 7.2AQ1

Results from time period:

FRI Jul 19 13:57:00 2019

FRI Jul 19 14:38:50 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0542	mg/l	7/19/2019 13:57:00	
0.1PPM	A	Phenolics-	P	0.0968	mg/l	7/19/2019 13:57:00	
0.25PPM	A	Phenolics-	P	0.2497	mg/l	7/19/2019 13:57:00	
0.50PPM	A	Phenolics-	P	0.5009	mg/l	7/19/2019 13:57:00	
1.0PPM	A	Phenolics-	P	0.9971	mg/l	7/19/2019 13:57:00	
2.0PPM	A	Phenolics-	P	2.0013	mg/l	7/19/2019 13:57:00	
ICV1	S	Phenolics-	P	1.014	mg/l	7/19/2019 14:26:00	
ICB1	S	Phenolics-	P	0.004	mg/l	7/19/2019 14:26:00	
CCV1	S	Phenolics-	P	1.001	mg/l	7/19/2019 14:26:00	
CCB1	S	Phenolics-	P	0.002	mg/l	7/19/2019 14:26:00	
PB121520BL	S	Phenolics-	P	0.002	mg/l	7/19/2019 14:26:00	
PB121520BS	S	Phenolics-	P	1.022	mg/l	7/19/2019 14:26:00	
K3834-15	S	Phenolics-	P	0.005	mg/l	7/19/2019 14:26:00	
K3834-15DUP	S	Phenolics-	P	0.003	mg/l	7/19/2019 14:26:00	
K3834-15MS	S	Phenolics-	P	0.967	mg/l	7/19/2019 14:26:00	
K3834-15MSD	S	Phenolics-	P	0.969	mg/l	7/19/2019 14:26:00	
K3882-01	S	Phenolics-	P	0.001	mg/l	7/19/2019 14:26:00	
K3883-01	S	Phenolics-	P	0.001	mg/l	7/19/2019 14:26:00	
K3905-01	S	Phenolics-	P	0.002	mg/l	7/19/2019 14:26:00	
K3908-01	S	Phenolics-	P	0.031	mg/l	7/19/2019 14:38:00	
CCV2	S	Phenolics-	P	0.999	mg/l	7/19/2019 14:38:00	
CCB2	S	Phenolics-	P	-0.004	mg/l	7/19/2019 14:38:00	