

LB104161

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : CT

Instrument ID : Konelab

7/23/2019 14:00

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.435	0.0	0.096	
ICB1	2.054	0.0	0.005	
CCV1	240.638	0.0	0.236	
CCB1	2.432	0.0	0.005	
PB121650BL	2.179	0.0	0.005	
PB121650BS	96.955	0.0	0.097	
LOWPB121650	9.656	0.0	0.012	
HIGHPB121650	485.231	0.0	0.474	
K3618-07	1.548	0.0	0.004	
K3618-07DUP	0.945	0.0	0.004	
K3618-07MS	37.038	0.0	0.039	
K3618-07MSD	38.775	0.0	0.041	
K3933-02	186.292	0.0	0.184	
K3835-25	0.298	0.0	0.003	
CCV2	251.007	0.0	0.246	
CCB2	-0.744	0.0	0.002	

N	16
Mean	90.609
SD	136.9187
CV%	151.11

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

7/23/2019 11:57


Test Total CN

Accepted 7/23/2019 11:57

Factor 1031
Bias 0.003

Coeff. of det. 0.999942

Errors

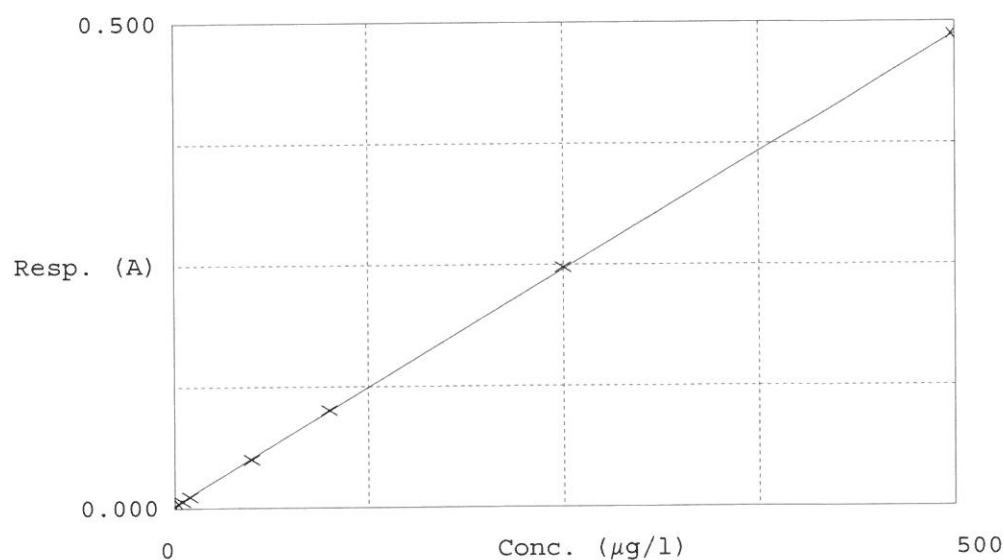

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	1.1573	0.0000	
2	5.0PPBCN	0.007	4.1281	5.0000	
3	10PPBCN	0.012	9.1718	10.0000	
4	50PPBCN	0.050	48.4516	50.0000	
5	100PPBCN	0.101	101.0912	100.0000	
6	250PPBCN	0.247	252.0763	250.0000	
7	500PPBCN	0.487	498.9238	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Tue Jul 23 11:24:54 2019

Tue Jul 23 13:49:54 2019

CT

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	1.1573	µg/l	7/23/2019 11:55:07	
5.0PPBCN	A	Total CN	P	4.1281	µg/l	7/23/2019 11:55:08	
10PPBCN	A	Total CN	P	9.1718	µg/l	7/23/2019 11:55:09	
50PPBCN	A	Total CN	P	48.4516	µg/l	7/23/2019 11:55:10	
100PPBCN	A	Total CN	P	101.0912	µg/l	7/23/2019 11:55:11	
250PPBCN	A	Total CN	P	252.0763	µg/l	7/23/2019 11:55:12	
500PPBCN	A	Total CN	P	498.9238	µg/l	7/23/2019 11:55:13	
ICV1	S	Total CN	P	95.435	µg/l	7/23/2019 12:47:13	
ICB1	S	Total CN	P	2.0539	µg/l	7/23/2019 12:47:14	
CCV1	S	Total CN	P	240.6376	µg/l	7/23/2019 12:47:15	
CCB1	S	Total CN	P	2.4321	µg/l	7/23/2019 12:47:16	
PB121650BL	S	Total CN	P	2.1793	µg/l	7/23/2019 12:47:18	
PB121650BS	S	Total CN	P	96.9549	µg/l	7/23/2019 12:47:19	
LOWPB121650	S	Total CN	P	9.6557	µg/l	7/23/2019 12:47:20	
HIGHPB121650	S	Total CN	P	485.2307	µg/l	7/23/2019 12:47:21	
K3618-07	S	Total CN	P	1.5479	µg/l	7/23/2019 12:47:22	
K3618-07DUP	S	Total CN	P	0.9451	µg/l	7/23/2019 12:47:23	
K3618-07MS	S	Total CN	P	37.0382	µg/l	7/23/2019 12:54:47	
K3618-07MSD	S	Total CN	P	38.7746	µg/l	7/23/2019 12:54:48	
K3933-02	S	Total CN	P	186.292	µg/l	7/23/2019 12:54:49	
K3835-25	S	Total CN	P	0.298	µg/l	7/23/2019 13:49:49	
CCV2	S	Total CN	P	251.0069	µg/l	7/23/2019 13:49:52	
CCB2	S	Total CN	P	-0.7435	µg/l	7/23/2019 13:49:53	