


LB104189

7470A

INSTRUMENT ID: CV1

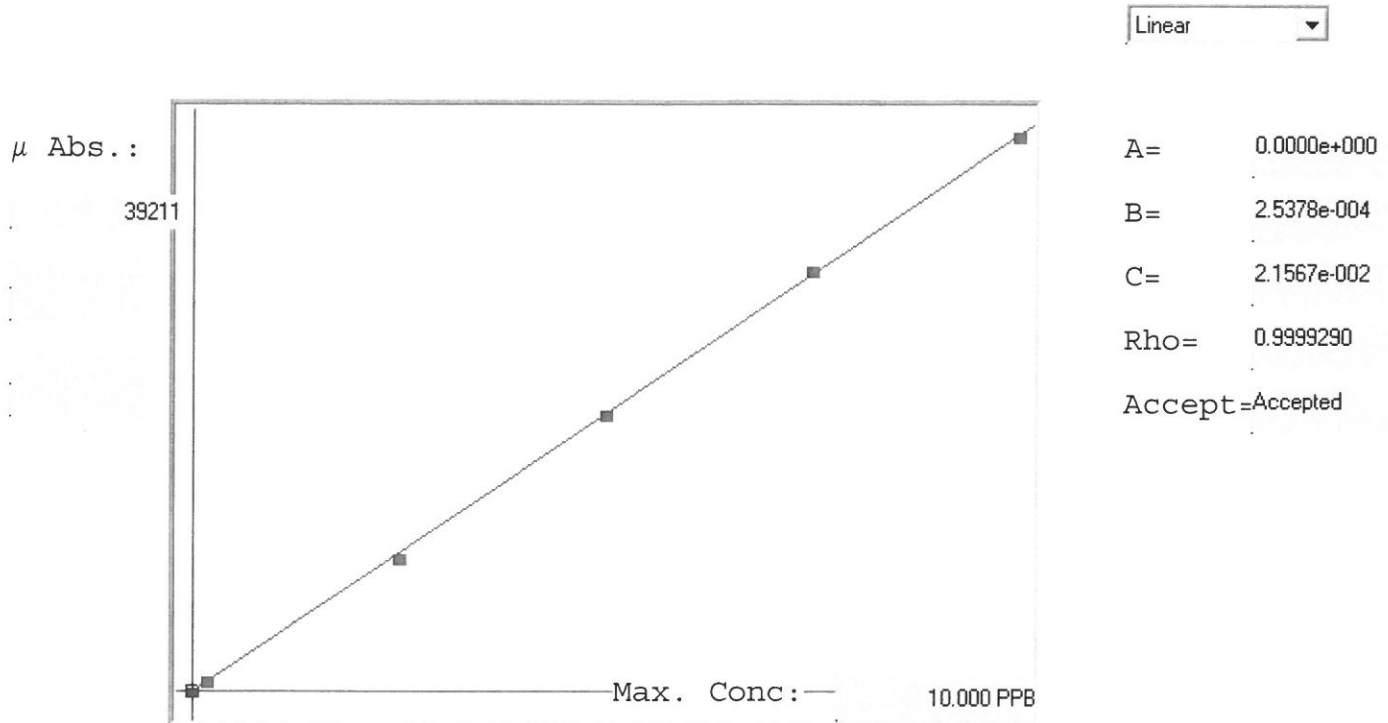

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.036	0.036	58	0.000	58				
0.2	0.200	0.207	0.007	732	0.0 %	732				
2.5	2.500	2.425	-0.075	9472	0.0 %	9472				
5.0	5.000	4.996	-0.004	19602	0.0 %	19602				
7.5	7.500	7.562	0.062	29714	0.0 %	29714				
10.0	10.000	9.973	-0.027	39211	0.0 %	39211				

LB104189 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 24 Jul 2019 14:11:53

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50-0	58	-	0.0007470A	PPB	24 Jul 2019 14:13:18	S	Std
0.2 - 1	50-2	732	-	0.20007470A	PPB	24 Jul 2019 14:15:26	S	Std
2.5 - 1	52-5	9472	-	2.50007470A	PPB	24 Jul 2019 14:17:36	S	Std
5.0 - 1	55-0	19602	-	5.00007470A	PPB	24 Jul 2019 14:19:44	S	Std
7.5 - 1	57-5	29714	-	7.50007470A	PPB	24 Jul 2019 14:21:52	S	Std
10.0 - 1	510-0	39211	-	10.00007470A	PPB	24 Jul 2019 14:37:17	S	Std
ICV45 - 1	ICV45	15244	3.8902	-7470A	PPB	24 Jul 2019 14:39:54	U	SMPL
ICB45 - 1	ICB45	27	0.0284	-7470A	PPB	24 Jul 2019 14:42:00	U	SMPL
CCV80 - 1	CCV80	19587	4.9923	-7470A	PPB	24 Jul 2019 14:44:06	U	SMPL
CCB80 - 1	CCB80	24	0.0277	-7470A	PPB	24 Jul 2019 14:46:12	U	SMPL
CRA - 1	CRA	722	0.2048	-7470A	PPB	24 Jul 2019 14:48:19	U	SMPL
HighStd - 1	HighStd	38961	9.9091	-7470A	PPB	24 Jul 2019 14:50:25	U	SMPL
ChkStd - 1	ChkStd	27069	6.8911	-7470A	PPB	24 Jul 2019 14:52:32	U	SMPL
PB121696BL - 1	PBW	-9	0.0193	-7470A	PPB	24 Jul 2019 14:54:40	U	SMPL
PB121696BS - 1	LCSW	14289	3.6478	-7470A	PPB	24 Jul 2019 14:56:47	U	SMPL
K3618-08 - 1	HD-02-072219	16	0.0256	-7470A	PPB	24 Jul 2019 14:58:56	U	SMPL
K3618-08DUP - 1	HD-02-072219DUP	35	0.0304	-7470A	PPB	24 Jul 2019 15:01:04	U	SMPL
K3618-08MS - 1	HD-02-072219MS	15907	4.0584	-7470A	PPB	24 Jul 2019 15:03:12	U	SMPL
K3618-08MSD - 1	HD-02-072219MSD	15334	3.9130	-7470A	PPB	24 Jul 2019 15:05:21	U	SMPL
K3940-01 - 1	A-7-22-19	10	0.0241	-7470A	PPB	24 Jul 2019 15:07:27	U	SMPL
CCV81 - 1	CCV81	19496	4.9692	-7470A	PPB	24 Jul 2019 15:09:34	U	SMPL
CCB81 - 1	CCB81	38	0.0312	-7470A	PPB	24 Jul 2019 15:11:40	U	SMPL
K3940-02 - 1	B-7-22-19	57	0.0360	-7470A	PPB	24 Jul 2019 15:13:47	U	SMPL
K3940-03 - 1	C-7-22-19	76	0.0409	-7470A	PPB	24 Jul 2019 15:15:54	U	SMPL
K3940-04 - 1	D-7-22-19	61	0.0370	-7470A	PPB	24 Jul 2019 15:18:01	U	SMPL
K3940-05 - 1	E-7-22-19	57	0.0360	-7470A	PPB	24 Jul 2019 15:20:08	U	SMPL
K3943-02 - 1	PA-71619	66	0.0383	-7470A	PPB	24 Jul 2019 15:22:15	U	SMPL
PB121697BL - 1	PBW	39	0.0315	-7470A	PPB	24 Jul 2019 15:24:22	U	SMPL
PB121697BS - 1	LCSW	14103	3.6006	-7470A	PPB	24 Jul 2019 15:26:31	U	SMPL
K3934-14 - 1	TP-1	28	0.0287	-7470A	PPB	24 Jul 2019 15:28:39	U	SMPL
K3934-17 - 1	TP-3	85	0.0431	-7470A	PPB	24 Jul 2019 15:30:47	U	SMPL
K3934-17DUP - 1	TP-3DUP	102	0.0475	-7470A	PPB	24 Jul 2019 15:32:54	U	SMPL
CCV82 - 1	CCV82	19240	4.9043	-7470A	PPB	24 Jul 2019 15:35:01	U	SMPL
CCB82 - 1	CCB82	-4	0.0206	-7470A	PPB	24 Jul 2019 15:37:07	U	SMPL
K3934-17MS - 1	TP-3MS	14782	3.7729	-7470A	PPB	24 Jul 2019 15:39:14	U	SMPL
K3934-17MSD - 1	TP-3MSD	16073	4.1006	-7470A	PPB	24 Jul 2019 15:41:22	U	SMPL
PB121698BL - 1	PBW	21	0.0269	-7470A	PPB	24 Jul 2019 15:43:29	U	SMPL
PB121698BS - 1	LCSW	14118	3.6044	-7470A	PPB	24 Jul 2019 15:45:36	U	SMPL
K3907-01 - 1	10-B	61	0.0370	-7470A	PPB	24 Jul 2019 15:47:43	U	SMPL
K3907-01DUP - 1	10-BDUP	99	0.0467	-7470A	PPB	24 Jul 2019 15:49:50	U	SMPL
K3907-01MS - 1	10-BMS	15098	3.8531	-7470A	PPB	24 Jul 2019 15:51:58	U	SMPL
K3907-01MSD - 1	10-BMSD	15965	4.0732	-7470A	PPB	24 Jul 2019 15:54:07	U	SMPL
PB121699BL - 1	PBW	34	0.0302	-7470A	PPB	24 Jul 2019 15:56:15	U	SMPL
PB121699BS - 1	LCSW	13962	3.5648	-7470A	PPB	24 Jul 2019 15:58:22	U	SMPL
CCV83 - 1	CCV83	19382	4.9403	-7470A	PPB	24 Jul 2019 16:00:29	U	SMPL
CCB83 - 1	CCB83	-6	0.0200	-7470A	PPB	24 Jul 2019 16:02:36	U	SMPL
K3591-07 - 1	LOD-MDL-WATER-01-QT3-2019	162	0.0627	-7470A	PPB	24 Jul 2019 16:04:43	U	SMPL
K3591-08 - 1	LOQ-WATER-02-QT3-2019	1524	0.4083	-7470A	PPB	24 Jul 2019 16:06:54	U	SMPL
PB121696TB - 1	PB121627TB	40	0.0317	-7470A	PPB	24 Jul 2019 16:09:04	U	SMPL
PB121697TB - 1	PB121629TB	50	0.0343	-7470A	PPB	24 Jul 2019 16:11:17	U	SMPL
PB121698TB - 1	PB121630TB	38	0.0312	-7470A	PPB	24 Jul 2019 16:13:24	U	SMPL
K3618-08LX5 - 1		0	0.0216	-7470A	PPB	24 Jul 2019 16:15:31	U	SMPL
K3618-08A - 1		15557	3.9696	-7470A	PPB	24 Jul 2019 16:17:38	U	SMPL
K3934-17LX5 - 1		15	0.0254	-7470A	PPB	24 Jul 2019 16:19:45	U	SMPL
K3934-17A - 1		15462	3.9455	-7470A	PPB	24 Jul 2019 16:21:52	U	SMPL
K3907-01LX5 - 1		-6	0.0200	-7470A	PPB	24 Jul 2019 16:24:00	U	SMPL
CCV84 - 1	CCV84	19333	4.9279	-7470A	PPB	24 Jul 2019 16:26:07	U	SMPL
CCB84 - 1	CCB84	-1	0.0213	-7470A	PPB	24 Jul 2019 16:28:14	U	SMPL
K3907-01A - 1		15029	3.8356	-7470A	PPB	24 Jul 2019 16:30:21	U	SMPL
CCV85 - 1	CCV85	19736	5.0302	-7470A	PPB	24 Jul 2019 16:32:28	U	SMPL
CCB85 - 1	CCB85	16	0.0256	-7470A	PPB	24 Jul 2019 16:34:35	U	SMPL