

LB104214

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : _____

Instrument ID : Konelab

7/25/2019 11:18


Test ~~Total~~ ^{Reactive} CN

Accepted 7/25/2019 11:18

Factor 1071
 Bias 0.002

Coeff. of det. 0.999966

Errors

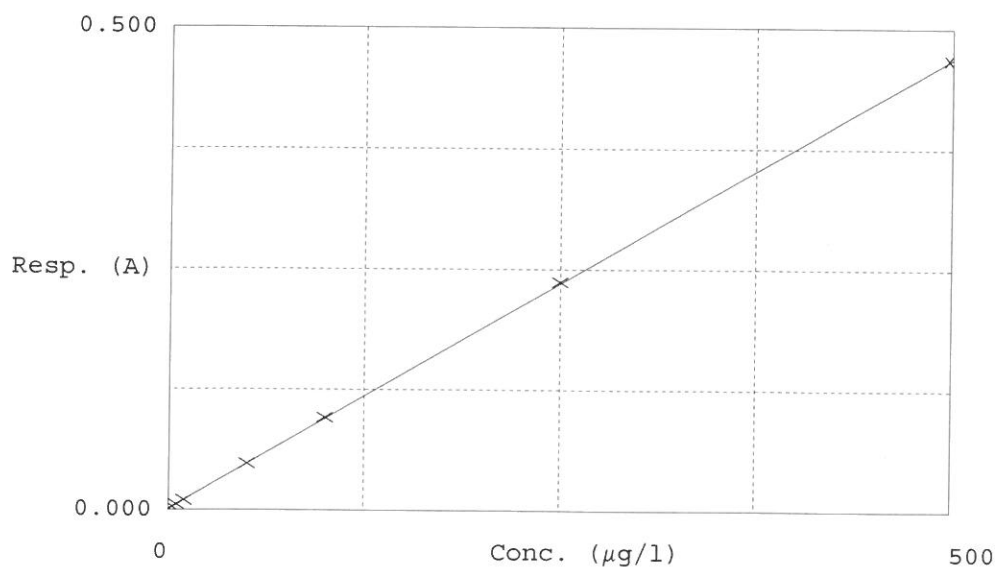

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.5092	0.0000	
2	5.0PPBCN	0.006	4.4802	5.0000	
3	10PPBCN	0.010	9.2473	10.0000	
4	50PPBCN	0.048	49.9468	50.0000	
5	100PPBCN	0.096	101.1131	100.0000	
6	250PPBCN	0.237	251.8377	250.0000	
7	500PPBCN	0.468	498.8841	500.0000	

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : CT

Instrument ID : Konelab

7/25/2019 13:28

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.462	0.0	0.092	
ICB1	0.121	0.0	0.002	
CCV1	243.970	0.0	0.229	
CCB1	-0.180	0.0	0.001	
PB121719BL	-0.359	0.0	0.001	
K3614-02	-0.504	0.0	0.001	
K3614-02DUP	-0.546	0.0	0.001	
K3961-04	-0.470	0.0	0.001	
PB121687BL	-0.130	0.0	0.001	
K3969-03	-0.164	0.0	0.001	
K3969-03DUP	-0.110	0.0	0.001	
CCV2	256.165	0.0	0.241	
CCB2	-0.204	0.0	0.001	

N	13
Mean	45.696
SD	94.5613
CV%	206.93

Aquakem v. 7.2AQ1

Results from time period:

Thu Jul 25 11:14:59 2019

Thu Jul 25 13:26:51 2019

CT

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.5092	µg/l	7/25/2019 11:14:59	
5.OPPBCN	A	Reactive CN	P	4.4802	µg/l	7/25/2019 11:15:00	
10PPBCN	A	Reactive CN	P	9.2473	µg/l	7/25/2019 11:15:01	
50PPBCN	A	Reactive CN	P	49.9468	µg/l	7/25/2019 11:15:02	
100PPBCN	A	Reactive CN	P	101.1131	µg/l	7/25/2019 11:15:03	
250PPBCN	A	Reactive CN	P	251.8377	µg/l	7/25/2019 11:15:04	
500PPBCN	A	Reactive CN	P	498.8841	µg/l	7/25/2019 11:15:05	
ICV1	S	Reactive CN	P	96.462	µg/l	7/25/2019 13:23:27	
ICB1	S	Reactive CN	P	0.121	µg/l	7/25/2019 13:23:28	
CCV1	S	Reactive CN	P	243.9703	µg/l	7/25/2019 13:23:29	
CCB1	S	Reactive CN	P	-0.1804	µg/l	7/25/2019 13:23:30	
PB121719BL	S	Reactive CN	P	-0.3585	µg/l	7/25/2019 13:23:31	
K3614-02	S	Reactive CN	P	-0.5041	µg/l	7/25/2019 13:23:32	
K3614-02DUP	S	Reactive CN	P	-0.5459	µg/l	7/25/2019 13:23:33	
K3961-04	S	Reactive CN	P	-0.47	µg/l	7/25/2019 13:23:34	
PB121687BL	S	Reactive CN	P	-0.1304	µg/l	7/25/2019 13:23:35	
K3969-03	S	Reactive CN	P	-0.1641	µg/l	7/25/2019 13:23:36	
K3969-03DUP	S	Reactive CN	P	-0.1102	µg/l	7/25/2019 13:23:37	
CCV2	S	Reactive CN	P	256.1653	µg/l	7/25/2019 13:26:50	
CCB2	S	Reactive CN	P	-0.2036	µg/l	7/25/2019 13:26:51	