

LB104264

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

7/26/2019 16:59

Test: ~~Total~~ ^{Reactive} CN

CT
07/26/19

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.510	0.0	0.089	
ICB1	0.193	0.0	0.002	
CCV1	237.355	0.0	0.224	
CCB1	-0.202	0.0	0.001	
PB121750BL	-0.248	0.0	0.001	
K3620-12	0.048	0.0	0.002	
K3620-12DUP	-0.656	0.0	0.001	
K3620-14	-0.475	0.0	0.001	
K3620-16	-0.290	0.0	0.001	
K3620-18	-0.441	0.0	0.001	
K3620-20	-0.307	0.0	0.001	
K3626-10	-0.187	0.0	0.001	
K3626-12	0.052	0.0	0.002	
K3626-14	0.260	0.0	0.002	
CCV2	237.558	0.0	0.224	
CCB2	-0.057	0.0	0.001	
K3626-16	-0.134	0.0	0.001	
K4012-01	-0.436	0.0	0.001	
K4012-04	0.034	0.0	0.002	
K4013-01	31.354	0.0	0.031	
CCV3	248.526	0.0	0.235	
CCB3	-0.219	0.0	0.001	

N	22
Mean	38.420
SD	85.0185
CV%	221.29

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : *CT*

Instrument ID : Konelab

7/26/2019 12:57


Test *Reactive*
~~Total~~ CN

Accepted 7/26/2019 12:56

Factor 1066
Bias 0.002

Coeff. of det. 0.999961

Errors

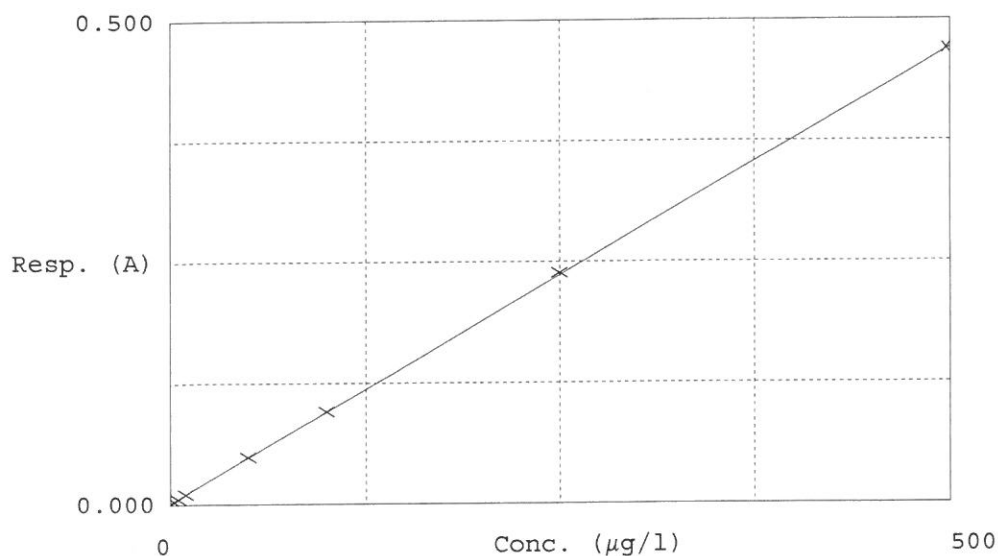

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.5377	0.0000	
2	5.0PPBCN	0.006	4.3909	5.0000	
3	10PPBCN	0.011	9.6079	10.0000	
4	50PPBCN	0.049	50.1907	50.0000	
5	100PPBCN	0.096	100.2074	100.0000	
6	250PPBCN	0.238	252.3748	250.0000	
7	500PPBCN	0.470	498.7661	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Fri Jul 26 16:33:22 2019

Fri Jul 26 16:58:29 2019

CT

Sample Id	Sam/Ctr/c/	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.5377	µg/l	7/26/2019 12:45:45	
5.0PPBCN	A	Reactive CN	P	4.3909	µg/l	7/26/2019 12:45:46	
10PPBCN	A	Reactive CN	P	9.6079	µg/l	7/26/2019 12:45:47	
50PPBCN	A	Reactive CN	P	50.1907	µg/l	7/26/2019 12:45:48	
100PPBCN	A	Reactive CN	P	100.2074	µg/l	7/26/2019 12:45:49	
250PPBCN	A	Reactive CN	P	252.3748	µg/l	7/26/2019 12:45:50	
500PPBCN	A	Reactive CN	P	498.7661	µg/l	7/26/2019 12:45:51	
ICV1	S	Reactive CN	P	93.51	µg/l	7/26/2019 16:33:22	
ICB1	S	Reactive CN	P	0.1925	µg/l	7/26/2019 16:33:23	
CCV1	S	Reactive CN	P	237.3545	µg/l	7/26/2019 16:33:24	
CCB1	S	Reactive CN	P	-0.2022	µg/l	7/26/2019 16:33:25	
PB121750E	S	Reactive CN	P	-0.2484	µg/l	7/26/2019 16:33:26	
K3620-12	S	Reactive CN	P	0.0482	µg/l	7/26/2019 16:33:27	
K3620-12D	S	Reactive CN	P	-0.656	µg/l	7/26/2019 16:33:28	
K3620-14	S	Reactive CN	P	-0.4753	µg/l	7/26/2019 16:33:29	
K3620-16	S	Reactive CN	P	-0.2905	µg/l	7/26/2019 16:33:30	
K3620-18	S	Reactive CN	P	-0.4414	µg/l	7/26/2019 16:33:31	
K3620-20	S	Reactive CN	P	-0.3074	µg/l	7/26/2019 16:33:32	
K3626-10	S	Reactive CN	P	-0.1867	µg/l	7/26/2019 16:40:57	
K3626-12	S	Reactive CN	P	0.0522	µg/l	7/26/2019 16:40:58	
K3626-14	S	Reactive CN	P	0.2602	µg/l	7/26/2019 16:40:59	
CCV2	S	Reactive CN	P	237.5578	µg/l	7/26/2019 16:41:00	
CCB2	S	Reactive CN	P	-0.0574	µg/l	7/26/2019 16:41:01	
K3626-16	S	Reactive CN	P	-0.1338	µg/l	7/26/2019 16:41:02	
K4012-01	S	Reactive CN	P	-0.4359	µg/l	7/26/2019 16:41:03	
K4012-04	S	Reactive CN	P	0.0344	µg/l	7/26/2019 16:41:04	
K4013-01	S	Reactive CN	P	31.3542	µg/l	7/26/2019 16:58:27	
CCV3	S	Reactive CN	P	248.5262	µg/l	7/26/2019 16:58:28	
CCB3	S	Reactive CN	P	-0.2195	µg/l	7/26/2019 16:58:29	