

7470A


LB104290

INSTRUMENT ID : CU1

Linear

 μ Abs.:

40857

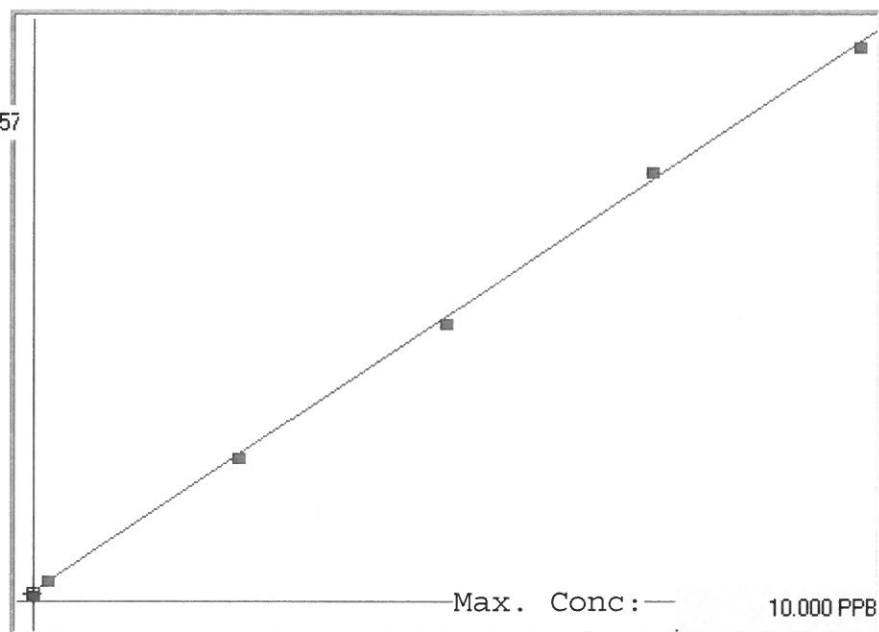

A= 0.0000e+000

B= 2.4700e-004

C= -1.6887e-001

Rho= 0.9997220

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.002	0.002	693	0.000	693				
0.2	0.200	0.230	0.030	1615	0.0 %	1615				
2.5	2.500	2.471	-0.029	10686	0.0 %	10686				
5.0	5.000	4.905	-0.095	20543	0.0 %	20543				
7.5	7.500	7.669	0.169	31734	0.0 %	31734				
10.0	10.000	9.923	-0.077	40857	0.0 %	40857				

Method: 7470A		Operator: Admin		Date of Analysis: 29 Jul 2019 13:46:22						
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units		Date	Type	Type
0.0 - 1	50-0	693	-	0.0000	7470A	PPB		29 Jul 2019	13:53:39	S Std
0.2 - 1	50-2	1615	-	0.2000	7470A	PPB		29 Jul 2019	13:55:48	S Std
2.5 - 1	52-5	10686	-	2.5000	7470A	PPB		29 Jul 2019	13:57:57	S Std
5.0 - 1	55-0	20543	-	5.0000	7470A	PPB		29 Jul 2019	14:00:05	S Std
7.5 - 1	57-5	31734	-	7.5000	7470A	PPB		29 Jul 2019	14:02:13	S Std
10.0 - 1	510-0	40857	-	10.0000	7470A	PPB		29 Jul 2019	14:04:20	S Std
ICV50 - 1	ICV50	17209	4.0817		7470A	PPB		29 Jul 2019	14:07:08	U SMPL
ICB50 - 1	ICB50	670	-0.0034		7470A	PPB		29 Jul 2019	14:09:15	U SMPL
CCV03 - 1	CCV03	20749	4.9561		7470A	PPB		29 Jul 2019	14:11:21	U SMPL
CCB03 - 1	CCB03	669	-0.0036		7470A	PPB		29 Jul 2019	14:13:28	U SMPL
CRA - 1	CRA	1632	0.2342		7470A	PPB		29 Jul 2019	14:15:35	U SMPL
HighStd - 1	HighStd	40723	9.8896		7470A	PPB		29 Jul 2019	14:17:41	U SMPL
ChkStd - 1	ChkStd	30017	7.2452		7470A	PPB		29 Jul 2019	14:19:48	U SMPL
PB121797BL - 1	PBW	405	-0.0688		7470A	PPB		29 Jul 2019	14:24:44	U SMPL
PB121797BS - 1	LCSW	15559	3.6741		7470A	PPB		29 Jul 2019	14:26:51	U SMPL
K4021-04 - 1	TP-10	176	-0.1254		7470A	PPB		29 Jul 2019	14:28:59	U SMPL
K4021-04DUP - 1	TP-10DUP	169	-0.1271		7470A	PPB		29 Jul 2019	14:32:54	U SMPL
K4021-04MS - 1	TP-10MS	16378	3.8764		7470A	PPB		29 Jul 2019	14:35:02	U SMPL
K4021-04MSD - 1	TP-10MSD	16864	3.9965		7470A	PPB		29 Jul 2019	14:37:10	U SMPL
K4021-08 - 1	TP-9	115	-0.1405		7470A	PPB		29 Jul 2019	14:39:17	U SMPL
CCV04 - 1	CCV04	21045	5.0292		7470A	PPB		29 Jul 2019	14:41:23	U SMPL
CCB04 - 1	CCB04	681	-0.0007		7470A	PPB		29 Jul 2019	14:43:30	U SMPL
K4021-12 - 1	TP-7	262	-0.1042		7470A	PPB		29 Jul 2019	14:45:37	U SMPL
K4021-16 - 1	TP-8-A	145	-0.1331		7470A	PPB		29 Jul 2019	14:47:43	U SMPL
K4024-04 - 1	TP-8	142	-0.1338		7470A	PPB		29 Jul 2019	14:49:50	U SMPL
K4024-08 - 1	TP-6-A	161	-0.1291		7470A	PPB		29 Jul 2019	14:51:57	U SMPL
PB121798BL - 1	PBW	165	-0.1281		7470A	PPB		29 Jul 2019	14:54:05	U SMPL
PB121798BS - 1	LCSW	15602	3.6848		7470A	PPB		29 Jul 2019	14:56:12	U SMPL
K4024-10 - 1	TP-8	117	-0.1400		7470A	PPB		29 Jul 2019	14:58:21	U SMPL
K4024-10DUP - 1	TP-8DUP	147	-0.1326		7470A	PPB		29 Jul 2019	15:00:31	U SMPL
K4024-10MS - 1	TP-8MS	16958	4.0197		7470A	PPB		29 Jul 2019	15:02:40	U SMPL
K4024-10MSD - 1	TP-8MSD	17034	4.0385		7470A	PPB		29 Jul 2019	15:04:47	U SMPL
CCV05 - 1	CCV05	20792	4.9667		7470A	PPB		29 Jul 2019	15:06:54	U SMPL
CCB05 - 1	CCB05	604	-0.0197		7470A	PPB		29 Jul 2019	15:09:01	U SMPL
PB121799BL - 1	PBW	168	-0.1274		7470A	PPB		29 Jul 2019	15:11:08	U SMPL
PB121799BS - 1	LCSW	15852	3.7465		7470A	PPB		29 Jul 2019	15:13:15	U SMPL
K3995-01 - 1	A1014	247	-0.1079		7470A	PPB		29 Jul 2019	15:15:21	U SMPL
K3995-01DUP - 1	A1014DUP	266	-0.1032		7470A	PPB		29 Jul 2019	15:17:28	U SMPL
K3995-01MS - 1	A1014MS	16323	3.8629		7470A	PPB		29 Jul 2019	15:19:36	U SMPL
K3995-01MSD - 1	A1014MSD	16946	4.0167		7470A	PPB		29 Jul 2019	15:21:43	U SMPL
K4024-09 - 1	TP-8	30521	7.3697		7470A	PPB		29 Jul 2019	15:23:51	U SMPL
K4036-01 - 1	WS-01	313	-0.0916		7470A	PPB		29 Jul 2019	15:25:59	U SMPL
K4036-02 - 1	WS-02	261	-0.1044		7470A	PPB		29 Jul 2019	15:28:08	U SMPL
K4036-03 - 1	WS-03	298	-0.0953		7470A	PPB		29 Jul 2019	15:30:15	U SMPL
CCV06 - 1	CCV06	20459	4.8844		7470A	PPB		29 Jul 2019	15:32:22	U SMPL
CCB06 - 1	CCB06	560	-0.0306		7470A	PPB		29 Jul 2019	15:34:29	U SMPL
K4036-04 - 1	WS-04	215	-0.1158		7470A	PPB		29 Jul 2019	15:36:35	U SMPL
PB121797TB - 1	PB121752TB	148	-0.1323		7470A	PPB		29 Jul 2019	16:01:11	U SMPL
PB121798TB - 1	PB121766TB	145	-0.1331		7470A	PPB		29 Jul 2019	16:03:18	U SMPL
K4021-04LX5 - 1		44	-0.1580		7470A	PPB		29 Jul 2019	16:05:26	U SMPL
K4021-04A - 1		16546	3.9179		7470A	PPB		29 Jul 2019	16:07:34	U SMPL
K4024-10LX5 - 1		0	-0.1689		7470A	PPB		29 Jul 2019	16:09:43	U SMPL
K4024-10A - 1		17089	4.0520		7470A	PPB		29 Jul 2019	16:11:50	U SMPL
CCV07 - 1	CCV07	20854	4.9820		7470A	PPB		29 Jul 2019	16:13:57	U SMPL
CCB07 - 1	CCB07	569	-0.0283		7470A	PPB		29 Jul 2019	16:16:05	U SMPL
K3995-01LX5 - 1		58	-0.1545		7470A	PPB		29 Jul 2019	16:18:12	U SMPL
K3995-01A - 1		16689	3.9533		7470A	PPB		29 Jul 2019	16:20:19	U SMPL
CCV08 - 1	CCV08	20832	4.9766		7470A	PPB		29 Jul 2019	16:22:25	U SMPL
CCB08 - 1	CCB08	633	-0.0125		7470A	PPB		29 Jul 2019	16:24:33	U SMPL