


LB104355

7470A

INSTRUMENT ID : CV1

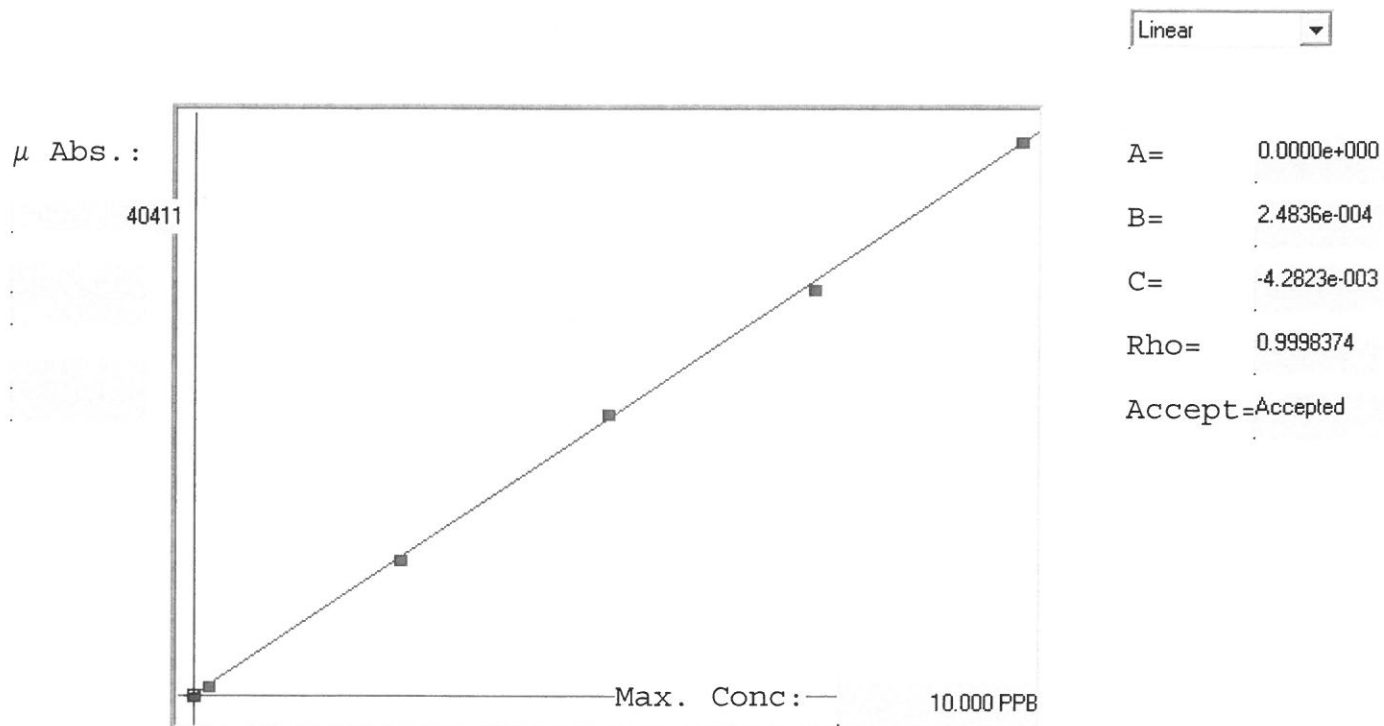

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.003	0.003	30	0.000	30				
0.2	0.200	0.183	-0.017	753	0.0 %	753				
2.5	2.500	2.487	-0.013	10032	0.0 %	10032				
5.0	5.000	5.109	0.109	20589	0.0 %	20589				
7.5	7.500	7.385	-0.115	29754	0.0 %	29754				
10.0	10.000	10.032	0.032	40411	0.0 %	40411				

LB104355 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 01 Aug 2019 11:02:45

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	30	-	0.0000	7470A	PPB	01 Aug 2019 11:22:47	S	Std
0.2 - 1	50.2	753	-	0.2000	7470A	PPB	01 Aug 2019 11:25:02	S	Std
2.5 - 1	52.5	10032	-	2.5000	7470A	PPB	01 Aug 2019 11:27:10	S	Std
5.0 - 1	55.0	20589	-	5.0000	7470A	PPB	01 Aug 2019 11:29:19	S	Std
7.5 - 1	57.5	29754	-	7.5000	7470A	PPB	01 Aug 2019 11:31:26	S	Std
10.0 - 1	510.0	40411	-	10.0000	7470A	PPB	01 Aug 2019 11:33:33	S	Std
ICV56 - 1	ICV56	17108	4.2447	-	7470A	PPB	01 Aug 2019 11:38:27	U	SMPL
ICB56 - 1	ICB56	-15	-0.0080	-	7470A	PPB	01 Aug 2019 11:40:33	U	SMPL
CCV30 - 1	CCV30	20891	5.1842	-	7470A	PPB	01 Aug 2019 11:42:41	U	SMPL
CCB30 - 1	CCB30	-27	-0.0110	-	7470A	PPB	01 Aug 2019 11:44:47	U	SMPL
CRA - 1	CRA	755	0.1832	-	7470A	PPB	01 Aug 2019 11:46:54	U	SMPL
HighStd - 1	HighStd	41871	10.3948	-	7470A	PPB	01 Aug 2019 11:49:00	U	SMPL
ChkStd - 1	ChkStd	30556	7.5846	-	7470A	PPB	01 Aug 2019 11:51:08	U	SMPL
PB121901BL - 1	PBW	0	0.0043	-	7470A	PPB	01 Aug 2019 11:53:14	U	SMPL
ChkStd - 1	ChkStd	28006	6.9513	-	7470A	PPB	01 Aug 2019 11:54:19	U	SMPL
PB121901BL - 1	PBW	-35	-0.0130	-	7470A	PPB	01 Aug 2019 11:56:26	U	SMPL
PB121901BS - 1	LCSW	15928	3.9516	-	7470A	PPB	01 Aug 2019 11:58:33	U	SMPL
K3618-10 - 1	HD-02-073019	19	0.0004	-	7470A	PPB	01 Aug 2019 12:00:40	U	SMPL
K3618-10DUP - 1	HD-02-073019DUP	35	0.0044	-	7470A	PPB	01 Aug 2019 12:02:48	U	SMPL
K3618-10MS - 1	HD-02-073019MS	16894	4.1915	-	7470A	PPB	01 Aug 2019 12:04:56	U	SMPL
K3618-10MSD - 1	HD-02-073019MSD	16557	4.1078	-	7470A	PPB	01 Aug 2019 12:07:05	U	SMPL
K4066-02 - 1	TP-1-A	25	0.0019	-	7470A	PPB	01 Aug 2019 12:09:11	U	SMPL
CCV31 - 1	CCV31	21530	5.3429	-	7470A	PPB	01 Aug 2019 12:11:18	U	SMPL
CCB31 - 1	CCB31	-14	-0.0078	-	7470A	PPB	01 Aug 2019 12:13:24	U	SMPL
K4066-08 - 1	TP-11	20	0.0007	-	7470A	PPB	01 Aug 2019 12:15:31	U	SMPL
K4066-12 - 1	TP-12	25	0.0019	-	7470A	PPB	01 Aug 2019 12:17:38	U	SMPL
K4066-16 - 1	TP-13	31	0.0034	-	7470A	PPB	01 Aug 2019 12:19:44	U	SMPL
K4074-11 - 1	SS-12_072919	39	0.0054	-	7470A	PPB	01 Aug 2019 12:21:51	U	SMPL
K4074-12 - 1	SS-11_072919	50	0.0081	-	7470A	PPB	01 Aug 2019 12:23:58	U	SMPL
K4077-02 - 1	20190612-LOC-13	16	-0.0003	-	7470A	PPB	01 Aug 2019 12:26:06	U	SMPL
PB121905BL - 1	PBW	37	0.0049	-	7470A	PPB	01 Aug 2019 12:28:13	U	SMPL
PB121905BS - 1	LCSW	15990	3.9670	-	7470A	PPB	01 Aug 2019 12:30:23	U	SMPL
K4110-01 - 1	190731-PUMP4	230	0.0528	-	7470A	PPB	01 Aug 2019 12:32:46	U	SMPL
K4110-01DUP - 1	190731-PUMP4DUP	169	0.0377	-	7470A	PPB	01 Aug 2019 12:34:53	U	SMPL
CCV32 - 1	CCV32	21443	5.3213	-	7470A	PPB	01 Aug 2019 12:36:59	U	SMPL
CCB32 - 1	CCB32	-23	-0.0100	-	7470A	PPB	01 Aug 2019 12:39:06	U	SMPL
K4110-01MS - 1	190731-PUMP4MS	15863	3.9355	-	7470A	PPB	01 Aug 2019 12:41:12	U	SMPL
K4110-01MSD - 1	190731-PUMP4MSD	16480	4.0887	-	7470A	PPB	01 Aug 2019 12:43:19	U	SMPL
PB121901TB - 1	PB121843TB	-19	-0.0090	-	7470A	PPB	01 Aug 2019 12:45:25	U	SMPL
K3618-10LX5 - 1		25	0.0019	-	7470A	PPB	01 Aug 2019 12:47:32	U	SMPL
K3618-10A - 1		16546	4.1051	-	7470A	PPB	01 Aug 2019 12:49:39	U	SMPL
K4110-01LX5 - 1		40	0.0057	-	7470A	PPB	01 Aug 2019 12:51:48	U	SMPL
K4110-01A - 1		17218	4.2720	-	7470A	PPB	01 Aug 2019 12:53:56	U	SMPL
CCV33 - 1	CCV33	21520	5.3404	-	7470A	PPB	01 Aug 2019 12:56:04	U	SMPL
CCB33 - 1	CCB33	-21	-0.0095	-	7470A	PPB	01 Aug 2019 12:58:13	U	SMPL