


LB104371

245.1

INSTRUMENT ID : CV1

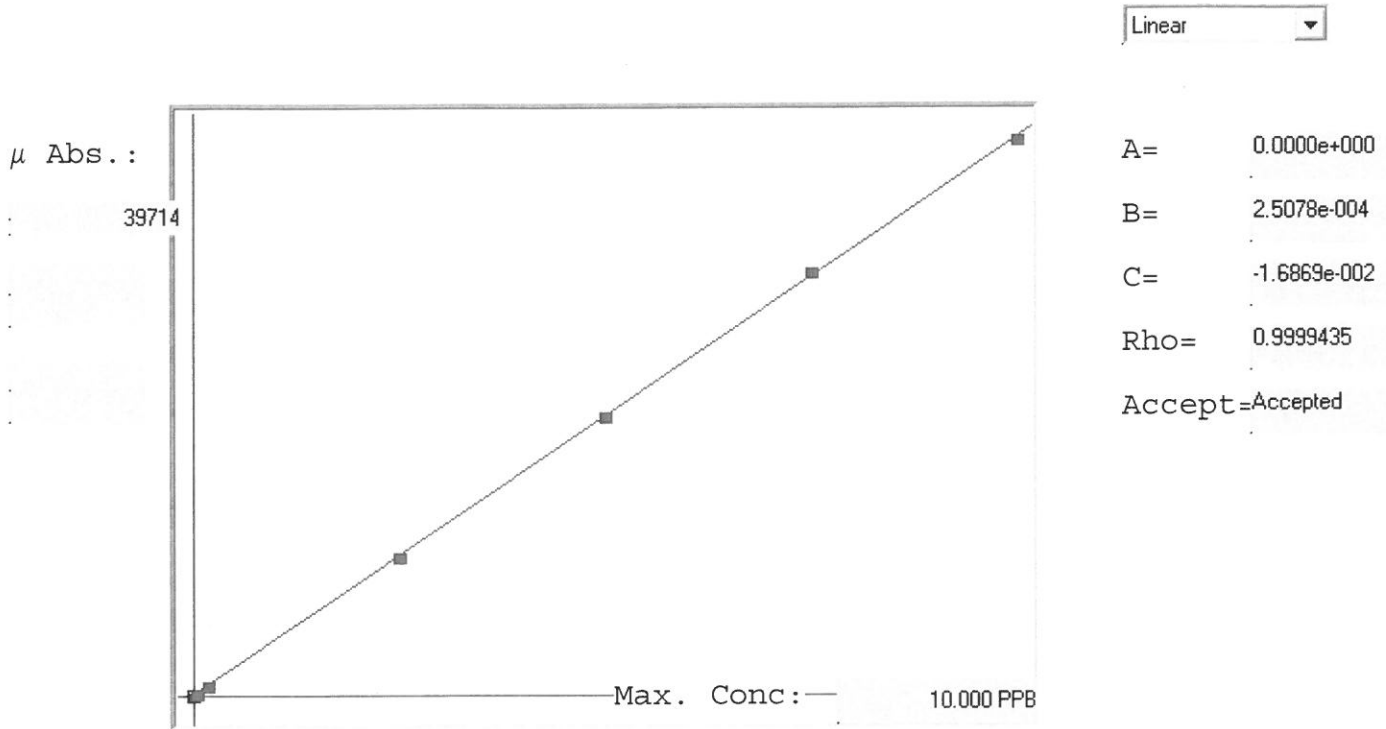

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.010	0.010	107	0.000	107				
0.05	0.050	0.049	-0.001	264	0.0 %	264				
0.2	0.200	0.181	-0.019	790	0.0 %	790				
2.5	2.500	2.490	-0.010	9998	0.0 %	9998				
5.0	5.000	4.993	-0.007	19977	0.0 %	19977				
7.5	7.500	7.584	0.084	30308	0.0 %	30308				
10.0	10.000	9.942	-0.058	39714	0.0 %	39714				

LB104371 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 01 Aug 2019 14:23:38

Sample ID	Extended ID	µ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50.0	107	-	0.0000245.1	PPB	01 Aug 2019 14:33:42	S	Std
0.05 - 1	50.05	264	-	0.0500245.1	PPB	01 Aug 2019 14:36:00	S	Std
0.2 - 1	50.2	790	-	0.2000245.1	PPB	01 Aug 2019 14:38:18	S	Std
2.5 - 1	52.5	9998	-	2.5000245.1	PPB	01 Aug 2019 14:40:36	S	Std
5.0 - 1	55.0	19977	-	5.0000245.1	PPB	01 Aug 2019 14:42:54	S	Std
7.5 - 1	57.5	30308	-	7.5000245.1	PPB	01 Aug 2019 14:45:11	S	Std
10.0 - 1	50.0	39714	-	10.0000245.1	PPB	01 Aug 2019 14:47:26	S	Std
ICV57 - 1	ICV57	15834	3.9539	-245.1	PPB	01 Aug 2019 14:58:43	U	SMPL
ICB57 - 1		17	-0.0126	-245.1	PPB	01 Aug 2019 15:00:59	U	SMPL
CCV34 - 1	CCV34	19803	4.9493	-245.1	PPB	01 Aug 2019 15:03:14	U	SMPL
CCB34 - 1	CCB34	40	-0.0068	-245.1	PPB	01 Aug 2019 15:05:30	U	SMPL
CRA - 1	CRA	264	0.0493	-245.1	PPB	01 Aug 2019 15:07:46	U	SMPL
HighStd - 1	HighStd	39814	9.9676	-245.1	PPB	01 Aug 2019 15:10:02	U	SMPL
ChkStd - 1	ChkStd	26931	6.7368	-245.1	PPB	01 Aug 2019 15:12:17	U	SMPL
PB121910BL - 1	PBW	-61	-0.0322	-245.1	PPB	01 Aug 2019 15:14:35	U	SMPL
PB121910BS - 1	LCSW	16867	4.2130	-245.1	PPB	01 Aug 2019 15:16:53	U	SMPL
K3992-01 - 1	55-ST-19	1	-0.0166	-245.1	PPB	01 Aug 2019 15:19:10	U	SMPL
K3992-01DUP - 1	55-ST-19DUP	35	-0.0081	-245.1	PPB	01 Aug 2019 15:21:27	U	SMPL
K3992-01MS - 1	55-ST-19MS	17043	4.2571	-245.1	PPB	01 Aug 2019 15:27:11	U	SMPL
K3992-01MSD - 1	55-ST-19MSD	17008	4.2483	-245.1	PPB	01 Aug 2019 15:29:28	U	SMPL
PB121911BL - 1	PBW	-8	-0.0189	-245.1	PPB	01 Aug 2019 15:31:44	U	SMPL
CCV35 - 1	CCV35	19330	4.8306	-245.1	PPB	01 Aug 2019 15:34:00	U	SMPL
CCB35 - 1	CCB35	41	-0.0066	-245.1	PPB	01 Aug 2019 15:36:16	U	SMPL
PB121911BS - 1	LCSW	16146	4.0322	-245.1	PPB	01 Aug 2019 15:38:32	U	SMPL
K3860-05 - 1	PT-HG-WS	14476	3.6134	-245.1	PPB	01 Aug 2019 15:40:48	U	SMPL
PB121912BL - 1	PBW	3	-0.0161	-245.1	PPB	01 Aug 2019 15:45:21	U	SMPL
PB121912BS - 1	LCSW	16314	4.0743	-245.1	PPB	01 Aug 2019 15:47:38	U	SMPL
K3591-12 - 1	MDL-MDL-WATER-06-QT3-2019	244	0.0443	-245.1	PPB	01 Aug 2019 15:53:25	U	SMPL
K3992-01LX5 - 1		-4	-0.0179	-245.1	PPB	01 Aug 2019 15:55:42	U	SMPL
K3992-01A - 1		17970	4.4896	-245.1	PPB	01 Aug 2019 15:57:59	U	SMPL
CCV36 - 1	CCV36	19277	4.8174	-245.1	PPB	01 Aug 2019 16:00:17	U	SMPL
CCB36 - 1	CCB36	47	-0.0051	-245.1	PPB	01 Aug 2019 16:04:02	U	SMPL