

LB104388

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

8/2/2019 10:07

Test: Total CN

ug/l

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.469	0.0	0.087	
ICB1	0.960	0.0	0.001	
CCV1	247.197	0.0	0.229	
CCB1	0.896	0.0	0.001	
PB121909BL	0.781	0.0	0.001	
PB121909BS	93.784	0.0	0.087	
LOWPB121909	10.894	0.0	0.011	
HIGHPB121909	485.985	0.0	0.449	
K4111-01	3.660	0.0	0.004	
K4111-01DUP	3.373	0.0	0.004	
K4111-01MSD	37.601	0.0	0.035	
K4111-01MS	38.099	0.0	0.036	
CCV2	249.377	0.0	0.231	
CCB2	1.154	0.0	0.002	
K4113-01	1.488	0.0	0.002	
K4114-01	2.998	0.0	0.003	
CCV3	251.032	0.0	0.232	
CCB3	1.285	0.0	0.002	

N	18
Mean	84.669
SD	135.9094
CV%	160.52

Aquakem v. 7.2AQ1

Results from time period:

Fri Aug 02 09:54:34 2019

Fri Aug 02 10:01:50 2019

CT

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.6612	µg/l	8/2/2019 8:29:16	
5.0PPBCN	A	Total CN	P	5.0991	µg/l	8/2/2019 8:29:17	
10PPBCN	A	Total CN	P	9.7776	µg/l	8/2/2019 8:29:18	
50PPBCN	A	Total CN	P	48.9795	µg/l	8/2/2019 8:29:19	
100PPBCN	A	Total CN	P	96.5023	µg/l	8/2/2019 8:29:20	
250PPBCN	A	Total CN	P	256.3504	µg/l	8/2/2019 8:29:21	
500PPBCN	A	Total CN	P	497.6299	µg/l	8/2/2019 8:29:22	
ICV1	S	Total CN	P	93.4692	µg/l	8/2/2019 9:54:34	
ICB1	S	Total CN	P	0.9604	µg/l	8/2/2019 9:54:35	
CCV1	S	Total CN	P	247.197	µg/l	8/2/2019 9:54:36	
CCB1	S	Total CN	P	0.8963	µg/l	8/2/2019 9:54:37	
PB121909BL	S	Total CN	P	0.7814	µg/l	8/2/2019 9:54:38	
PB121909BS	S	Total CN	P	93.7845	µg/l	8/2/2019 9:54:39	
LOWPB121909	S	Total CN	P	10.8936	µg/l	8/2/2019 9:54:40	
HIGHPB121909	S	Total CN	P	485.985	µg/l	8/2/2019 9:54:41	
K4111-01	S	Total CN	P	3.6595	µg/l	8/2/2019 9:54:42	
K4111-01DUP	S	Total CN	P	3.3734	µg/l	8/2/2019 9:54:43	
K4111-01MSD	S	Total CN	P	37.6009	µg/l	8/2/2019 10:01:42	
K4111-01MS	S	Total CN	P	38.0994	µg/l	8/2/2019 10:01:43	
CCV2	S	Total CN	P	249.3772	µg/l	8/2/2019 10:01:44	
CCB2	S	Total CN	P	1.1537	µg/l	8/2/2019 10:01:45	
K4113-01	S	Total CN	P	1.4885	µg/l	8/2/2019 10:01:46	
K4114-01	S	Total CN	P	2.9983	µg/l	8/2/2019 10:01:47	
CCV3	S	Total CN	P	251.0316	µg/l	8/2/2019 10:01:48	
CCB3	S	Total CN	P	1.2851	µg/l	8/2/2019 10:01:49	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

8/2/2019 8:31


Test Total CN

Accepted 8/2/2019 8:31

Factor 1084
Bias 0.001

Coeff. of det. 0.999710

Errors

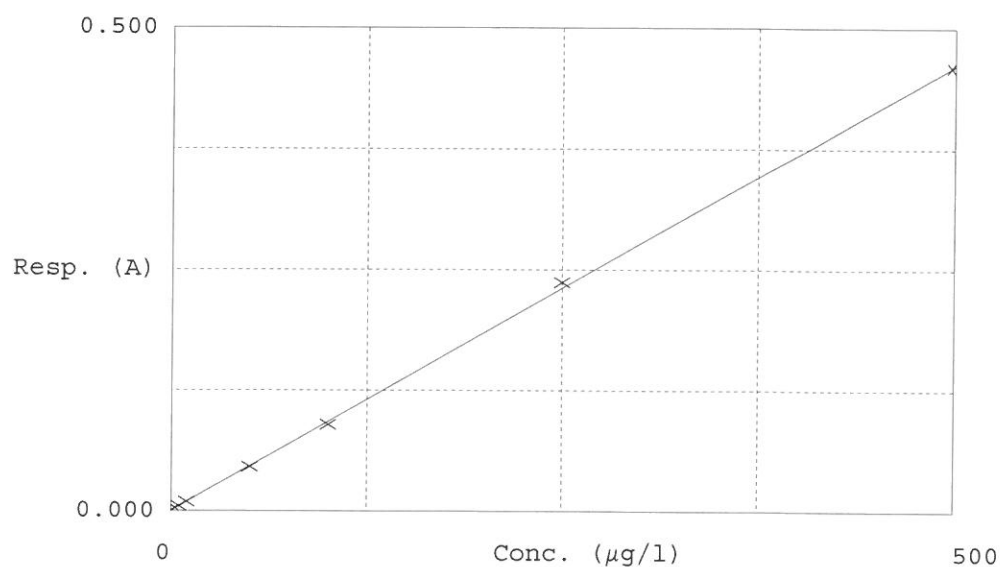

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.6612	0.0000	
2	5.0PPBCN	0.005	5.0991	5.0000	
3	10PPBCN	0.010	9.7776	10.0000	
4	50PPBCN	0.046	48.9795	50.0000	
5	100PPBCN	0.090	96.5023	100.0000	
6	250PPBCN	0.237	256.3504	250.0000	
7	500PPBCN	0.459	497.6299	500.0000	