


LB104392

7470A

INSTRUMENT ID : CU1

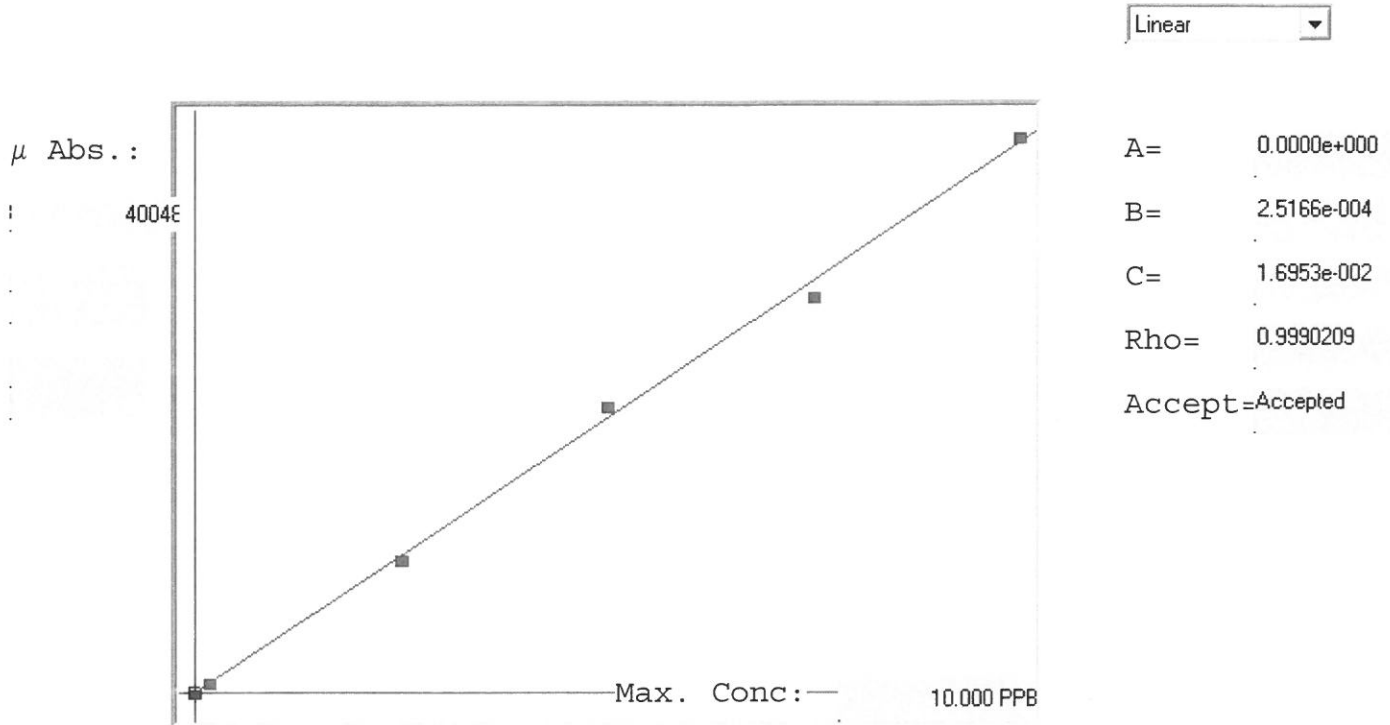

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.021	0.021	16	0.000	16				
0.2	0.200	0.199	-0.001	722	0.0 %	722				
2.5	2.500	2.426	-0.074	9574	0.0 %	9574				
5.0	5.000	5.248	0.248	20785	0.0 %	20785				
7.5	7.500	7.211	-0.289	28586	0.0 %	28586				
10.0	10.000	10.095	0.095	40048	0.0 %	40048				

LB104392 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 02 Aug 2019 11:44:47					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	16	-	0.0000	7470A	PPB	02 Aug 2019 11:49:03	S	Std
0.2 - 1	50-2	722	-	0.2000	7470A	PPB	02 Aug 2019 11:51:12	S	Std
2.5 - 1	52-5	9574	-	2.5000	7470A	PPB	02 Aug 2019 11:53:20	S	Std
5.0 - 1	55-0	20785	-	5.0000	7470A	PPB	02 Aug 2019 11:55:29	S	Std
7.5 - 1	57-5	28586	-	7.5000	7470A	PPB	02 Aug 2019 12:00:19	S	Std
10.0 - 1	50-0	40048	-	10.0000	7470A	PPB	02 Aug 2019 12:02:26	S	Std
ICV58 - 1	ICV58	17091	4.3181	-	7470A	PPB	02 Aug 2019 12:09:42	U	SMPL
ICB58 - 1	ICB58	-19	0.0122	-	7470A	PPB	02 Aug 2019 12:11:48	U	SMPL
CCV37 - 1	CCV37	20875	5.2704	-	7470A	PPB	02 Aug 2019 12:17:38	U	SMPL
CCB37 - 1	CCB37	6	0.0185	-	7470A	PPB	02 Aug 2019 12:19:44	U	SMPL
CRA - 1	CRA	766	0.2097	-	7470A	PPB	02 Aug 2019 12:21:51	U	SMPL
HighStd - 1	HighStd	41179	10.3801	-	7470A	PPB	02 Aug 2019 12:23:57	U	SMPL
ChkStd - 1	ChkStd	28469	7.1815	-	7470A	PPB	02 Aug 2019 12:26:04	U	SMPL
PB121936BL - 1	PBW	-41	0.0066	-	7470A	PPB	02 Aug 2019 12:28:11	U	SMPL
PB121936BS - 1	LCSW	16971	4.2879	-	7470A	PPB	02 Aug 2019 12:30:18	U	SMPL
K4106-02 - 1	WC-01	-11	0.0142	-	7470A	PPB	02 Aug 2019 12:32:25	U	SMPL
K4106-02DUP - 1	WC-01DUP	35	0.0258	-	7470A	PPB	02 Aug 2019 12:34:33	U	SMPL
K4106-02MS - 1	WC-01MS	16051	4.0563	-	7470A	PPB	02 Aug 2019 12:36:42	U	SMPL
K4106-02MSD - 1	WC-01MSD	15522	3.9232	-	7470A	PPB	02 Aug 2019 12:38:50	U	SMPL
PB121937BL - 1	PBW	17	0.0212	-	7470A	PPB	02 Aug 2019 12:40:56	U	SMPL
CCV38 - 1	CCV38	20119	5.0801	-	7470A	PPB	02 Aug 2019 12:43:03	U	SMPL
CCB38 - 1	CCB38	9	0.0192	-	7470A	PPB	02 Aug 2019 12:45:10	U	SMPL
PB121937BS - 1	LCSW	16962	4.2856	-	7470A	PPB	02 Aug 2019 12:47:17	U	SMPL
K4066-17 - 1	TP-13	38321	9.6608	-	7470A	PPB	02 Aug 2019 12:49:23	U	SMPL
K4111-01 - 1	P001-RB2-190731	-89	-0.0054	-	7470A	PPB	02 Aug 2019 12:51:30	U	SMPL
K4113-01 - 1	P001-RB01-190730	4	0.0180	-	7470A	PPB	02 Aug 2019 12:53:38	U	SMPL
K4114-01 - 1	CS-TEST-PIT	11188	2.8325	-	7470A	PPB	02 Aug 2019 12:55:45	U	SMPL
K4114-01DUP - 1	CS-TEST-PITDUP	11280	2.8557	-	7470A	PPB	02 Aug 2019 12:57:53	U	SMPL
K4114-01MS - 1	CS-TEST-PITMS	27214	6.8656	-	7470A	PPB	02 Aug 2019 13:00:01	U	SMPL
K4114-01MSD - 1	CS-TEST-PITMSD	24990	6.3059	-	7470A	PPB	02 Aug 2019 13:02:09	U	SMPL
PB121938BL - 1	PBW	-30	0.0094	-	7470A	PPB	02 Aug 2019 13:04:23	U	SMPL
PB121938BS - 1	LCSW	16784	4.2408	-	7470A	PPB	02 Aug 2019 13:06:28	U	SMPL
CCV39 - 1	CCV39	20252	5.1136	-	7470A	PPB	02 Aug 2019 13:08:34	U	SMPL
CCB39 - 1	CCB39	1	0.0172	-	7470A	PPB	02 Aug 2019 13:10:42	U	SMPL
K4066-18 - 1	TP-13	34	0.0255	-	7470A	PPB	02 Aug 2019 13:12:48	U	SMPL
K4066-18DUP - 1	TP-13DUP	29	0.0243	-	7470A	PPB	02 Aug 2019 13:14:55	U	SMPL
K4066-18MS - 1	TP-13MS	15677	3.9622	-	7470A	PPB	02 Aug 2019 13:17:02	U	SMPL
K4066-18MSD - 1	TP-13MSD	15876	4.0123	-	7470A	PPB	02 Aug 2019 13:19:08	U	SMPL
K4114-02 - 1	CS-TEST-PIT	15	0.0207	-	7470A	PPB	02 Aug 2019 13:21:16	U	SMPL
K4126-01 - 1	26-WARD-UNK-LIQUID	66686	16.7991	-	7470A	PPB	02 Aug 2019 13:23:23	U	SMPL
PB121936TB - 1	PB121880TB	-257	-0.0477	-	7470A	PPB	02 Aug 2019 13:30:11	U	SMPL
PB121938TB - 1	PB121913TB	-111	-0.0110	-	7470A	PPB	02 Aug 2019 13:32:19	U	SMPL
K4106-02LX5 - 1		-61	0.0016	-	7470A	PPB	02 Aug 2019 13:34:27	U	SMPL
K4106-02A - 1		16045	4.0548	-	7470A	PPB	02 Aug 2019 13:36:34	U	SMPL
CCV40 - 1	CCV40	19520	4.9294	-	7470A	PPB	02 Aug 2019 13:38:41	U	SMPL
CCB40 - 1	CCB40	-65	0.0006	-	7470A	PPB	02 Aug 2019 13:40:47	U	SMPL
K4114-01LX5 - 1		2109	0.5477	-	7470A	PPB	02 Aug 2019 13:42:54	U	SMPL
K4114-01A - 1		26371	6.6535	-	7470A	PPB	02 Aug 2019 13:45:01	U	SMPL
K4066-18LX5 - 1		-108	-0.0102	-	7470A	PPB	02 Aug 2019 13:47:08	U	SMPL
K4066-18A - 1		15929	4.0256	-	7470A	PPB	02 Aug 2019 13:49:16	U	SMPL
K4126-01DLX5 - 1		14633	3.6995	-	7470A	PPB	02 Aug 2019 14:50:42	U	SMPL
CCV41 - 1	CCV41	19427	4.9059	-	7470A	PPB	02 Aug 2019 14:52:49	U	SMPL
CCB41 - 1	CCB41	-34	0.0084	-	7470A	PPB	02 Aug 2019 14:54:57	U	SMPL