


LB104401

7471B

INSTRUMENT ID: CV1

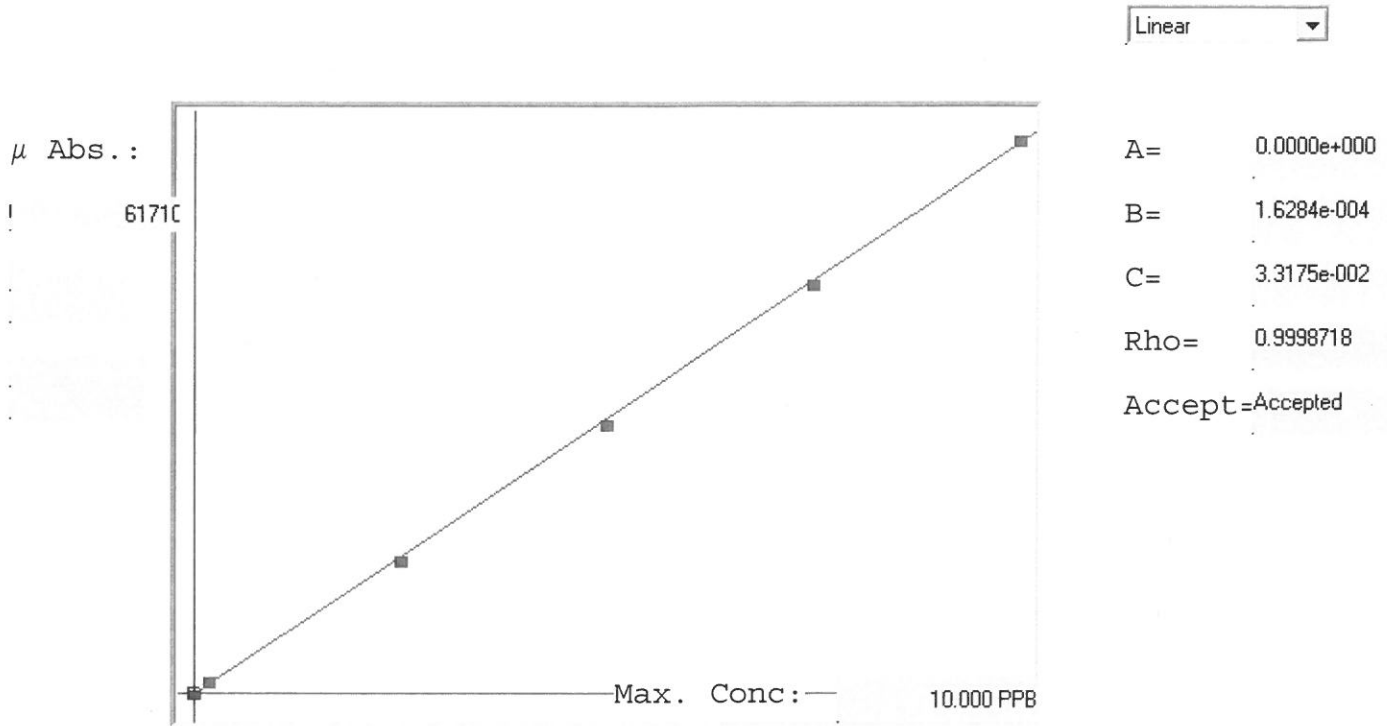

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.032	0.032	-7	0.000	-7				
0.2	0.200	0.250	0.050	1334	0.0 %	1334				
2.5	2.500	2.467	-0.033	14947	0.0 %	14947				
5.0	5.000	4.913	-0.087	29966	0.0 %	29966				
7.5	7.500	7.456	-0.044	45581	0.0 %	45581				
10.0	10.000	10.082	0.082	61710	0.0 %	61710				

LB104401 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 02 Aug 2019 15:13:43

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	-7	-	0.0000	7471B	PPB	02 Aug 2019 15:14:57	S	Std
0.2 - 1	50-2	1334	-	0.2000	7471B	PPB	02 Aug 2019 15:17:15	S	Std
2.5 - 1	52-5	14947	-	2.5000	7471B	PPB	02 Aug 2019 15:19:33	S	Std
5.0 - 1	55-0	29966	-	5.0000	7471B	PPB	02 Aug 2019 15:21:51	S	Std
7.5 - 1	57-5	45581	-	7.5000	7471B	PPB	02 Aug 2019 15:24:08	S	Std
10.0 - 1	57-6	61710	-	10.0000	7471B	PPB	02 Aug 2019 15:36:38	S	Std
ICV59 - 1	ICV59	23078	3.7912	-7471B	PPB	PPB	02 Aug 2019 15:41:00	U	SMPL
ICB59 - 1	ICB59	-59	0.0236	-7471B	PPB	PPB	02 Aug 2019 15:43:16	U	SMPL
CCV42 - 1	CCV42	29532	4.8422	-7471B	PPB	PPB	02 Aug 2019 15:45:32	U	SMPL
CCB42 - 1	CCB42	-60	0.0234	-7471B	PPB	PPB	02 Aug 2019 15:47:47	U	SMPL
CRA - 1	CRA	1328	0.2494	-7471B	PPB	PPB	02 Aug 2019 15:50:03	U	SMPL
HighStd - 1	HighStd	61223	10.0027	-7471B	PPB	PPB	02 Aug 2019 15:52:19	U	SMPL
ChkStd - 1	ChkStd	41352	6.7669	-7471B	PPB	PPB	02 Aug 2019 15:54:35	U	SMPL
PB121940BL - 1	PBS	-8	0.0319	-7471B	PPB	PPB	02 Aug 2019 15:56:53	U	SMPL
PB121940BS - 1	LCSS	21823	3.5868	-7471B	PPB	PPB	02 Aug 2019 15:59:10	U	SMPL
K4093-01 - 1	PL-02-080119	2023	0.3626	-7471B	PPB	PPB	02 Aug 2019 16:01:27	U	SMPL
K4093-01DUP - 1	PL-02-080119DUP	2025	0.3629	-7471B	PPB	PPB	02 Aug 2019 16:03:44	U	SMPL
K4093-01MS - 1	PL-02-080119MS	25578	4.1983	-7471B	PPB	PPB	02 Aug 2019 16:11:08	U	SMPL
K4093-01MSD - 1	PL-02-080119MSD	25471	4.1809	-7471B	PPB	PPB	02 Aug 2019 16:13:25	U	SMPL
K4106-01 - 1	WC-01	11318	1.8762	-7471B	PPB	PPB	02 Aug 2019 16:15:42	U	SMPL
CCV43 - 1	CCV43	29239	4.7944	-7471B	PPB	PPB	02 Aug 2019 16:17:58	U	SMPL
CCB43 - 1	CCB43	26	0.0374	-7471B	PPB	PPB	02 Aug 2019 16:20:14	U	SMPL
K4107-01 - 1	T-1	3641	0.6261	-7471B	PPB	PPB	02 Aug 2019 16:22:30	U	SMPL
K4107-03 - 1	T-2	2870	0.5005	-7471B	PPB	PPB	02 Aug 2019 16:24:45	U	SMPL
K4124-01 - 1	TP-15	17365	2.8609	-7471B	PPB	PPB	02 Aug 2019 16:27:01	U	SMPL
K4093-01LX5 - 1		352	0.0905	-7471B	PPB	PPB	02 Aug 2019 16:29:17	U	SMPL
K4093-01A - 1		23446	3.8511	-7471B	PPB	PPB	02 Aug 2019 16:31:34	U	SMPL
CCV44 - 1	CCV44	29509	4.8384	-7471B	PPB	PPB	02 Aug 2019 16:33:50	U	SMPL
CCB44 - 1	CCB44	-49	0.0252	-7471B	PPB	PPB	02 Aug 2019 16:36:08	U	SMPL