

LB104422

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : CT

Instrument ID : Konelab

8/5/2019 9:06


Test ^{Reactive}
~~Total~~ CN

Accepted 8/5/2019 9:06

Factor 1040
 Bias 0.002

Coeff. of det. 0.999982

Errors

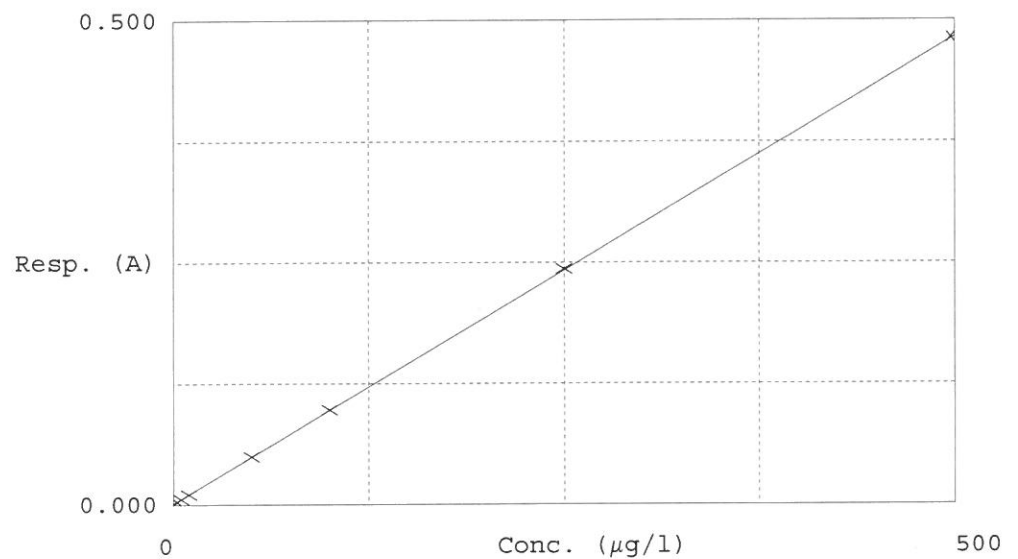

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.4108	0.0000	
2	5.0PPBCN	0.006	4.6001	5.0000	
3	10PPBCN	0.011	9.6363	10.0000	
4	50PPBCN	0.050	50.1421	50.0000	
5	100PPBCN	0.098	100.3289	100.0000	
6	250PPBCN	0.244	251.5440	250.0000	
7	500PPBCN	0.482	499.1592	500.0000	

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : CT

Instrument ID : Konelab

8/5/2019 9:54

Test: ^{Reactive} ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.532	0.0	0.093	
ICB1	-2.126	0.0	-0.001	
CCV1	241.907	0.0	0.234	
CCB1	-0.146	0.0	0.001	
PB12130BL	-0.249	0.0	0.001	
K4114-02	-0.417	0.0	0.001	
K4114-02DUP	-0.481	0.0	0.001	
PB121928BL	-0.208	0.0	0.001	
K4093-02	-0.343	0.0	0.001	
K4093-02DUP	-0.376	0.0	0.001	
K4124-02	-0.383	0.0	0.001	
CCV2	256.941	0.0	0.249	
CCB2	-0.160	0.0	0.001	

N	13
Mean	45.346
SD	94.4010
CV%	208.18

CT
08/5/19

Aquakem v. 7.2AQ1

Results from time period:

Mon Aug 05 08:27:58 2019

Mon Aug 05 09:27:51 2019



Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.4108	µg/l	8/5/2019 8:46:52	
5.OPPBCN	A	Reactive CN	P	4.6001	µg/l	8/5/2019 8:46:53	
10PPBCN	A	Reactive CN	P	9.6363	µg/l	8/5/2019 8:46:54	
50PPBCN	A	Reactive CN	P	50.1421	µg/l	8/5/2019 8:46:55	
100PPBCN	A	Reactive CN	P	100.3289	µg/l	8/5/2019 8:46:56	
250PPBCN	A	Reactive CN	P	251.544	µg/l	8/5/2019 8:46:57	
500PPBCN	A	Reactive CN	P	499.1592	µg/l	8/5/2019 8:46:58	
ICV1	S	Reactive CN	P	95.5323	µg/l	8/5/2019 9:24:27	
ICB1	S	Reactive CN	P	-2.1257	µg/l	8/5/2019 9:24:28	
CCV1	S	Reactive CN	P	241.9073	µg/l	8/5/2019 9:24:29	
CCB1	S	Reactive CN	P	-0.1457	µg/l	8/5/2019 9:24:30	
PB12130BL	S	Reactive CN	P	-0.2485	µg/l	8/5/2019 9:24:31	
K4114-02	S	Reactive CN	P	-0.4167	µg/l	8/5/2019 9:24:32	
K4114-02DUP	S	Reactive CN	P	-0.4811	µg/l	8/5/2019 9:24:33	
PB121928BL	S	Reactive CN	P	-0.2076	µg/l	8/5/2019 9:24:34	
K4093-02	S	Reactive CN	P	-0.3426	µg/l	8/5/2019 9:24:35	
K4093-02DUP	S	Reactive CN	P	-0.3764	µg/l	8/5/2019 9:24:36	
K4124-02	S	Reactive CN	P	-0.3827	µg/l	8/5/2019 9:24:37	
CCV2	S	Reactive CN	P	256.9409	µg/l	8/5/2019 9:27:50	
CCB2	S	Reactive CN	P	-0.1601	µg/l	8/5/2019 9:27:51	