


LB104484

7470A

INSTRUMENT ID: C01

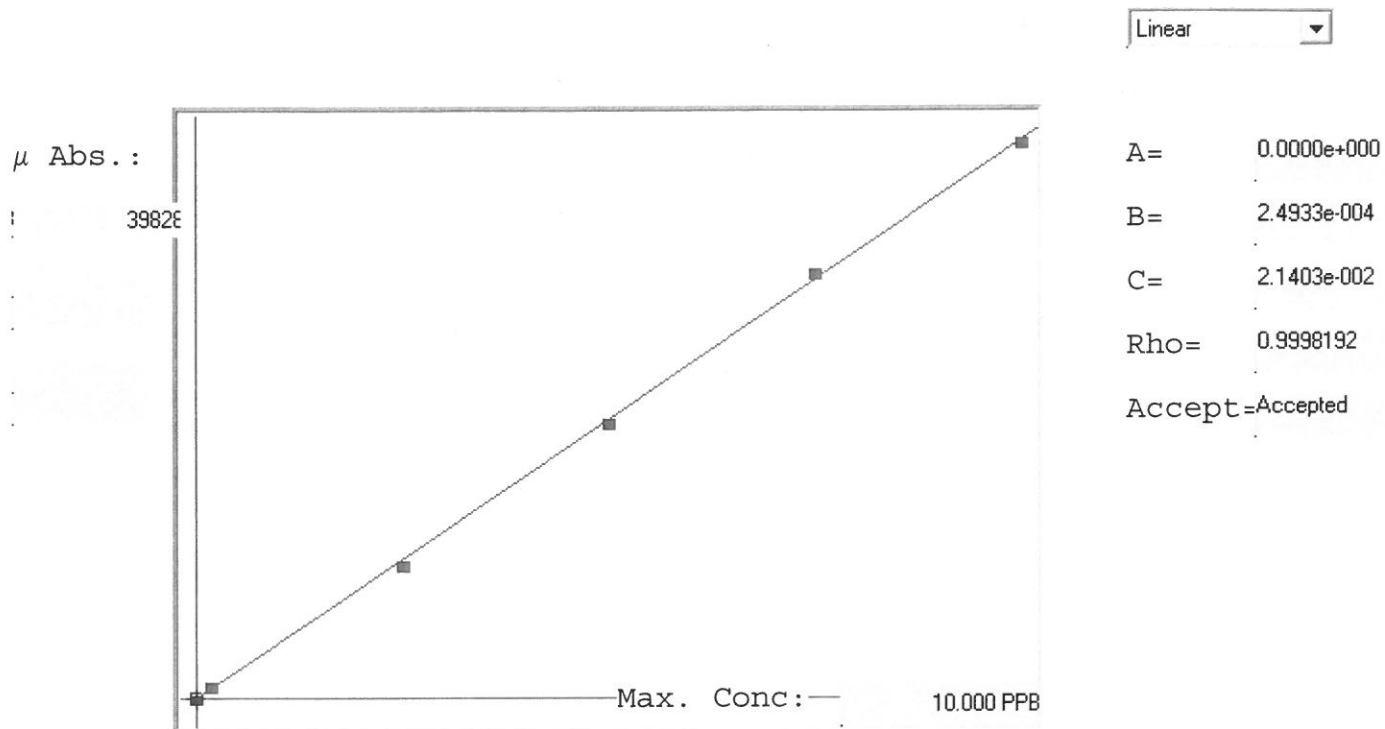

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.038	0.038	66	0.000	66				
0.2	0.200	0.228	0.028	828	0.0 %	828				
2.5	2.500	2.406	-0.094	9564	0.0 %	9564				
5.0	5.000	4.957	-0.043	19794	0.0 %	19794				
7.5	7.500	7.620	0.120	30474	0.0 %	30474				
10.0	10.000	9.952	-0.048	39828	0.0 %	39828				

LB104448 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 08 Aug 2019 10:20:37				
Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50.0	66	-	0.00007470A	PPB	08 Aug 2019 10:27:19	S	Std
0.2 - 1	50.2	828	-	0.20007470A	PPB	08 Aug 2019 10:29:28	S	Std
2.5 - 1	52.5	9564	-	2.50007470A	PPB	08 Aug 2019 10:31:37	S	Std
5.0 - 1	55.0	19794	-	5.00007470A	PPB	08 Aug 2019 10:33:45	S	Std
7.5 - 1	57.5	30474	-	7.50007470A	PPB	08 Aug 2019 10:35:54	S	Std
10.0 - 1	510.0	39828	-	10.00007470A	PPB	08 Aug 2019 10:40:47	S	Std
ICV63 - 1	ICV63	15577	3.9053	-7470A	PPB	08 Aug 2019 10:48:21	U	SMPL
ICB63 - 1	ICB63	15	0.0251	-7470A	PPB	08 Aug 2019 10:50:28	U	SMPL
CCV70 - 1	CCV70	19523	4.8892	-7470A	PPB	08 Aug 2019 10:52:35	U	SMPL
CCB70 - 1	CCB70	103	0.0471	-7470A	PPB	08 Aug 2019 10:54:41	U	SMPL
CRA - 1	CRA	829	0.2281	-7470A	PPB	08 Aug 2019 10:56:47	U	SMPL
HighStd - 1	HighStd	39220	9.8003	-7470A	PPB	08 Aug 2019 10:58:54	U	SMPL
ChkStd - 1	ChkStd	27720	6.9330	-7470A	PPB	08 Aug 2019 11:01:00	U	SMPL
PB122072BL - 1	PBW	-2	0.0209	-7470A	PPB	08 Aug 2019 11:03:07	U	SMPL
PB122072BS - 1	LCSW	16052	4.0237	-7470A	PPB	08 Aug 2019 11:05:15	U	SMPL
K4174-02 - 1	VW-PAINT-CHIPS	58	0.0359	-7470A	PPB	08 Aug 2019 11:07:22	U	SMPL
K4178-04 - 1	370-371	83	0.0421	-7470A	PPB	08 Aug 2019 11:09:30	U	SMPL
K4192-03 - 1	TRIPLE-BARREL-BC-WEST	170	0.0638	-7470A	PPB	08 Aug 2019 11:11:38	U	SMPL
K4192-05 - 1	TRIPLE-BARREL-BC-EAST	170	0.0638	-7470A	PPB	08 Aug 2019 11:13:47	U	SMPL
K4192-05DUP - 1	TRIPLE-BARREL-BC-EASTDUP	161	0.0615	-7470A	PPB	08 Aug 2019 11:15:54	U	SMPL
CCV71 - 1	CCV71	19542	4.8939	-7470A	PPB	08 Aug 2019 11:18:00	U	SMPL
CCB71 - 1	CCB71	66	0.0379	-7470A	PPB	08 Aug 2019 11:20:07	U	SMPL
K4192-05MS - 1	TRIPLE-BARREL-BC-EASTMS	15900	3.9858	-7470A	PPB	08 Aug 2019 11:27:08	U	SMPL
K4192-05MSD - 1	TRIPLE-BARREL-BC-EASTMSD	16118	4.0402	-7470A	PPB	08 Aug 2019 11:29:14	U	SMPL
PB122073BL - 1	PBW	19	0.0261	-7470A	PPB	08 Aug 2019 11:31:22	U	SMPL
PB122073BS - 1	LCSW	15781	3.9562	-7470A	PPB	08 Aug 2019 11:33:29	U	SMPL
K4190-04 - 1	30320	300	0.0962	-7470A	PPB	08 Aug 2019 11:35:36	U	SMPL
K4190-04DUP - 1	30320DUP	313	0.0994	-7470A	PPB	08 Aug 2019 11:37:44	U	SMPL
K4190-04MS - 1	30320MS	14704	3.6876	-7470A	PPB	08 Aug 2019 11:39:51	U	SMPL
K4190-04MSD - 1	30320MSD	14222	3.5674	-7470A	PPB	08 Aug 2019 11:42:00	U	SMPL
PB122072TB - 1	PB122025TB	-14	0.0179	-7470A	PPB	08 Aug 2019 11:44:09	U	SMPL
PB122073TB - 1	PB122029TB	34	0.0299	-7470A	PPB	08 Aug 2019 11:46:16	U	SMPL
CCV72 - 1	CCV72	19582	4.9039	-7470A	PPB	08 Aug 2019 11:48:22	U	SMPL
CCB72 - 1	CCB72	78	0.0409	-7470A	PPB	08 Aug 2019 11:50:29	U	SMPL
K4192-05LX5 - 1		38	0.0309	-7470A	PPB	08 Aug 2019 11:52:35	U	SMPL
K4192-05A - 1		15670	3.9285	-7470A	PPB	08 Aug 2019 11:54:42	U	SMPL
K4190-04LX5 - 1		73	0.0396	-7470A	PPB	08 Aug 2019 11:56:49	U	SMPL
K4190-04A - 1		14982	3.7569	-7470A	PPB	08 Aug 2019 12:00:59	U	SMPL
CCV73 - 1	CCV73	19590	4.9059	-7470A	PPB	08 Aug 2019 12:03:06	U	SMPL
CCB73 - 1	CCB73	14	0.0249	-7470A	PPB	08 Aug 2019 12:05:14	U	SMPL