


LB104510

7471B

INSTRUMENT ID : CU1

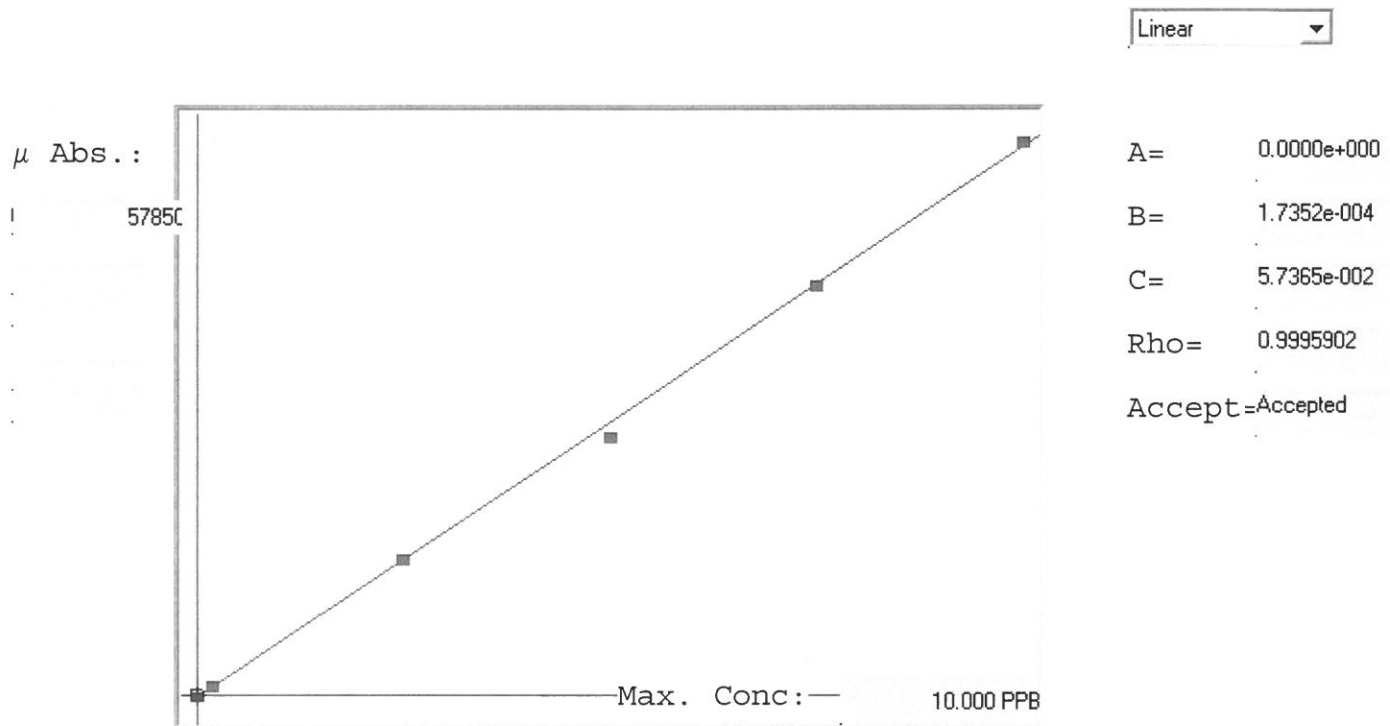

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.062	0.062	29	0.000	29				
0.2	0.200	0.236	0.036	1030	0.0 %	1030				
2.5	2.500	2.529	0.029	14242	0.0 %	14242				
5.0	5.000	4.772	-0.228	27173	0.0 %	27173				
7.5	7.500	7.505	0.005	42919	0.0 %	42919				
10.0	10.000	10.096	0.096	57850	0.0 %	57850				

LB104511 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 09 Aug 2019 12:47:39

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50.0	29	-	0.00007471B	PPB	09 Aug 2019 12:54:35	S	Std
0.2 - 1	50.2	1030	-	0.20007471B	PPB	09 Aug 2019 12:56:53	S	Std
2.5 - 1	52.5	14242	-	2.50007471B	PPB	09 Aug 2019 12:59:10	S	Std
5.0 - 1	55.0	27173	-	5.00007471B	PPB	09 Aug 2019 13:01:28	S	Std
7.5 - 1	57.5	42919	-	7.50007471B	PPB	09 Aug 2019 13:03:45	S	Std
10.0 - 1	510.0	57850	-	10.00007471B	PPB	09 Aug 2019 13:06:02	S	Std
ICV65 - 1	ICV65	22910	4.0328	-7471B	PPB	09 Aug 2019 13:09:17	U	SMPL
ICB65 - 1	ICB65	-49	0.0489	-7471B	PPB	09 Aug 2019 13:11:33	U	SMPL
CCV80 - 1	CCV80	28411	4.9873	-7471B	PPB	09 Aug 2019 13:13:49	U	SMPL
CCB80 - 1	CCB80	-56	0.0476	-7471B	PPB	09 Aug 2019 13:16:04	U	SMPL
CRA - 1	CRA	1027	0.2356	-7471B	PPB	09 Aug 2019 13:18:21	U	SMPL
HighStd - 1	HighStd	58244	10.1640	-7471B	PPB	09 Aug 2019 13:20:37	U	SMPL
ChkStd - 1	ChkStd	40459	7.0779	-7471B	PPB	09 Aug 2019 13:22:53	U	SMPL
PB122121BL - 1	PBS	-68	0.0456	-7471B	PPB	09 Aug 2019 13:25:10	U	SMPL
PB122121BS - 1	LCSS	21700	3.8228	-7471B	PPB	09 Aug 2019 13:27:27	U	SMPL
K4238-01 - 1	TP-17	12378	2.2052	-7471B	PPB	09 Aug 2019 13:29:44	U	SMPL
K4238-01DUP - 1	TP-17DUP	12284	2.1889	-7471B	PPB	09 Aug 2019 13:32:01	U	SMPL
K4238-01MS - 1	TP-17MS	37236	6.5186	-7471B	PPB	09 Aug 2019 13:34:19	U	SMPL
K4238-01MSD - 1	TP-17MSD	35121	6.1516	-7471B	PPB	09 Aug 2019 13:36:36	U	SMPL
K4238-05 - 1	TP-18	26735	4.6965	-7471B	PPB	09 Aug 2019 13:38:53	U	SMPL
CCV81 - 1	CCV81	28509	5.0043	-7471B	PPB	09 Aug 2019 13:41:10	U	SMPL
CCB81 - 1	CCB81	-65	0.0461	-7471B	PPB	09 Aug 2019 13:43:26	U	SMPL
K4241-01 - 1	TOTOWA-SOIL	915	0.2161	-7471B	PPB	09 Aug 2019 13:45:43	U	SMPL
K4244-01 - 1	BERGEN-SP-1	3933	0.7398	-7471B	PPB	09 Aug 2019 13:47:59	U	SMPL
K4244-03 - 1	BERGEN-SP-2	6193	1.1320	-7471B	PPB	09 Aug 2019 13:50:15	U	SMPL
K4245-01 - 1	COMP-25	14036	2.4929	-7471B	PPB	09 Aug 2019 13:52:31	U	SMPL
K4245-03 - 1	COMP-26	15074	2.6730	-7471B	PPB	09 Aug 2019 13:54:48	U	SMPL
K4245-05 - 1	COMP-27	17070	3.0194	-7471B	PPB	09 Aug 2019 13:57:04	U	SMPL
K4254-01 - 1	RECOVERED-CRSH-AGGREGATE-A	115	0.0773	-7471B	PPB	09 Aug 2019 13:59:21	U	SMPL
K4254-02 - 1	RECOVERED-CRSH-AGGREGATE-B	3917	0.7371	-7471B	PPB	09 Aug 2019 14:01:38	U	SMPL
K4254-03 - 1	RECOVERED-CRSH-AGGREGATE-C	513	0.1464	-7471B	PPB	09 Aug 2019 14:03:57	U	SMPL
K4257-01 - 1	SAND-A	2216	0.4419	-7471B	PPB	09 Aug 2019 14:06:12	U	SMPL
CCV82 - 1	CCV82	28539	5.0095	-7471B	PPB	09 Aug 2019 14:08:28	U	SMPL
CCB82 - 1	CCB82	-25	0.0530	-7471B	PPB	09 Aug 2019 14:10:44	U	SMPL
K4257-02 - 1	SAND-B	2594	0.5075	-7471B	PPB	09 Aug 2019 14:13:00	U	SMPL
K4270-01 - 1	FRONT-PROPERTY-2ND-BARN	3181	0.6093	-7471B	PPB	09 Aug 2019 14:15:16	U	SMPL
K4270-02 - 1	EXTRA-PROPERTY	2459	0.4841	-7471B	PPB	09 Aug 2019 14:17:32	U	SMPL
K4270-03 - 1	REAR-PROPERTY-2ND-BARN	1839	0.3765	-7471B	PPB	09 Aug 2019 14:19:48	U	SMPL
K4270-04 - 1	MIDDLE-PROPERTY-2ND-BARN	2938	0.5672	-7471B	PPB	09 Aug 2019 14:22:04	U	SMPL
PB122122BL - 1	PBS	-7	0.0562	-7471B	PPB	09 Aug 2019 14:24:21	U	SMPL
PB122122BS - 1	LCSS	21771	3.8351	-7471B	PPB	09 Aug 2019 14:26:38	U	SMPL
K4227-21 - 1	1S-I-(0-1)-COMP	2908	0.5620	-7471B	PPB	09 Aug 2019 14:28:55	U	SMPL
K4228-12 - 1	2S-I1-I4-COMP-(0-1)	4610	0.8573	-7471B	PPB	09 Aug 2019 14:31:13	U	SMPL
K4230-29 - 1	REACTOR-3A-(0-3)-COMP	7757	1.4034	-7471B	PPB	09 Aug 2019 14:33:29	U	SMPL
CCV83 - 1	CCV83	28236	4.9569	-7471B	PPB	09 Aug 2019 14:35:44	U	SMPL
CCB83 - 1	CCB83	-27	0.0527	-7471B	PPB	09 Aug 2019 14:38:00	U	SMPL
K4236-01 - 1	20190644	7096	1.2887	-7471B	PPB	09 Aug 2019 14:40:17	U	SMPL
K4236-02 - 1	20190645	2307	0.4577	-7471B	PPB	09 Aug 2019 14:42:33	U	SMPL
K4236-03 - 1	20190646	7095	1.2885	-7471B	PPB	09 Aug 2019 14:44:49	U	SMPL
K4237-01 - 1	SB-04(14-15)	2305	0.4573	-7471B	PPB	09 Aug 2019 14:49:22	U	SMPL
K4237-03 - 1	SB-05(0-2)	5671	1.0414	-7471B	PPB	09 Aug 2019 14:51:38	U	SMPL
K4237-04 - 1	SB-05(13-14)	1632	0.3406	-7471B	PPB	09 Aug 2019 14:53:55	U	SMPL
K4237-04DUP - 1	SB-05(13-14)DUP	1669	0.3470	-7471B	PPB	09 Aug 2019 14:56:13	U	SMPL
K4237-05 - 1	K4237-04MS	23140	4.0727	-7471B	PPB	09 Aug 2019 14:58:30	U	SMPL
K4237-06 - 1	K4237-04MSD	23479	4.1315	-7471B	PPB	09 Aug 2019 15:00:47	U	SMPL
CCV84 - 1	CCV84	28298	4.9677	-7471B	PPB	09 Aug 2019 15:03:03	U	SMPL
CCB84 - 1	CCB84	-25	0.0530	-7471B	PPB	09 Aug 2019 15:05:19	U	SMPL
K4237-07 - 1	SB-07(13-14)	318	0.1125	-7471B	PPB	09 Aug 2019 15:07:36	U	SMPL
K4237-08 - 1	DUP-X	1708	0.3537	-7471B	PPB	09 Aug 2019 15:09:52	U	SMPL
K4238-01LX5 - 1		2430	0.4790	-7471B	PPB	09 Aug 2019 15:12:08	U	SMPL
K4238-01A - 1		36599	6.4081	-7471B	PPB	09 Aug 2019 15:14:25	U	SMPL
K4237-04LX5 - 1		330	0.1146	-7471B	PPB	09 Aug 2019 15:16:41	U	SMPL
K4237-04A - 1		23469	4.1298	-7471B	PPB	09 Aug 2019 15:18:58	U	SMPL
CCV85 - 1	CCV85	28189	4.9488	-7471B	PPB	09 Aug 2019 15:21:15	U	SMPL
CCB85 - 1	CCB85	58	0.0674	-7471B	PPB	09 Aug 2019 15:23:34	U	SMPL