

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

8/12/2019 10:16


Test Total CN

Accepted 8/12/2019 10:16

Factor 1053
Bias 0.001

Coeff. of det. 0.999965

Errors

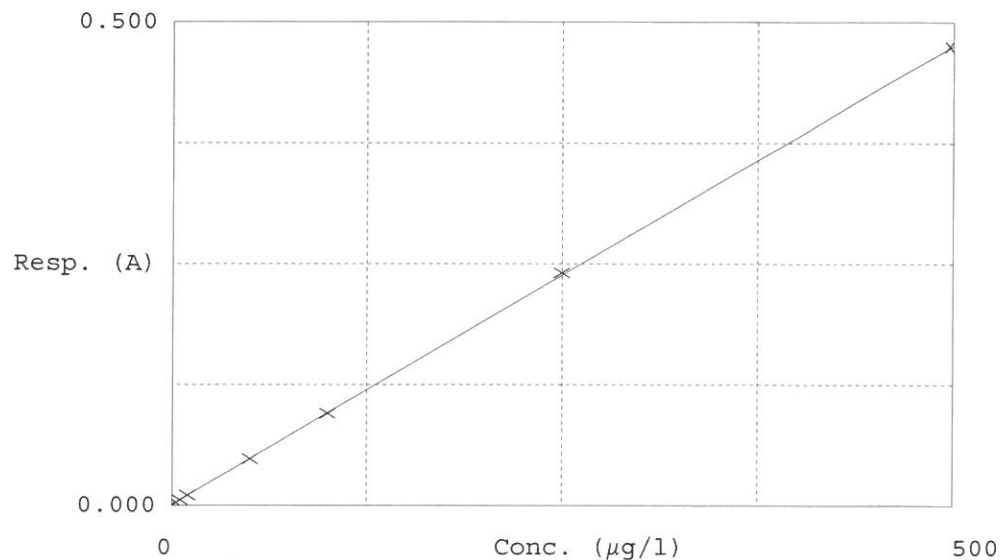

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.1229	0.0000	
2	5.0PPBCN	0.006	4.8671	5.0000	
3	10PPBCN	0.011	9.9906	10.0000	
4	50PPBCN	0.048	49.6514	50.0000	
5	100PPBCN	0.095	99.2587	100.0000	
6	250PPBCN	0.241	252.3408	250.0000	
7	500PPBCN	0.475	499.0142	500.0000	

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

8/12/2019 13:39

Test: Total CN

ug/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.022	0.0	0.091	
ICB1	0.637	0.0	0.002	
CCV1	242.359	0.0	0.231	
CCB1	0.609	0.0	0.002	
PB122135BL	9.786	0.0	0.010	
PB122135BS	0.640	0.0	0.002	
MIDPB122135	241.686	0.0	0.231	
K4263-02	0.281	0.0	0.001	
K4263-02DUP	0.319	0.0	0.001	
K4263-02MS	65.212	0.0	0.063	
K4263-02MSD	65.250	0.0	0.063	
K4271-01	1.114	0.0	0.002	
PB122135BL	0.137	0.0	0.001	
PB122135BS	100.939	0.0	0.097	
CCV2	255.144	0.0	0.243	
CCB2	0.613	0.0	0.002	

N 16
Mean 67.484
SD 95.6414
CV% 141.72

CT
8/12/19

Aquakem v. 7.2AQ1

CT

Results from time period:

Mon Aug 12 12:53:52 2019

Mon Aug 12 13:28:36 2019

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.1229	µg/l	8/12/2019 10:13:26	
5.0PPBCN	A	Total CN	P	4.8671	µg/l	8/12/2019 10:13:27	
10PPBCN	A	Total CN	P	9.9906	µg/l	8/12/2019 10:13:28	
50PPBCN	A	Total CN	P	49.6514	µg/l	8/12/2019 10:13:29	
100PPBCN	A	Total CN	P	99.2587	µg/l	8/12/2019 10:13:30	
250PPBCN	A	Total CN	P	252.3408	µg/l	8/12/2019 10:13:31	
500PPBCN	A	Total CN	P	499.0142	µg/l	8/12/2019 10:13:32	
ICV1	S	Total CN	P	95.0215	µg/l	8/12/2019 12:53:52	
ICB1	S	Total CN	P	0.637	µg/l	8/12/2019 12:53:55	
CCV1	S	Total CN	P	242.3594	µg/l	8/12/2019 12:53:56	
CCB1	S	Total CN	P	0.6094	µg/l	8/12/2019 12:53:59	
MIDPB122135	S	Total CN	P	241.6857	µg/l	8/12/2019 12:54:02	
K4263-02	S	Total CN	P	0.2807	µg/l	8/12/2019 13:00:03	
K4263-02DUP	S	Total CN	P	0.3186	µg/l	8/12/2019 13:00:04	
K4263-02MS	S	Total CN	P	65.212	µg/l	8/12/2019 13:00:05	
K4263-02MSD	S	Total CN	P	65.2498	µg/l	8/12/2019 13:00:06	
K4271-01	S	Total CN	P	1.1137	µg/l	8/12/2019 13:00:07	
PB122135BL	S	Total CN	P	0.1367	µg/l	8/12/2019 13:28:31	
PB122135BS	S	Total CN	P	100.9392	µg/l	8/12/2019 13:28:32	
CCV2	S	Total CN	P	255.1436	µg/l	8/12/2019 13:28:35	
CCB2	S	Total CN	P	0.6132	µg/l	8/12/2019 13:28:36	