


LB104587

7471B

INSTRUMENT ID : CV1

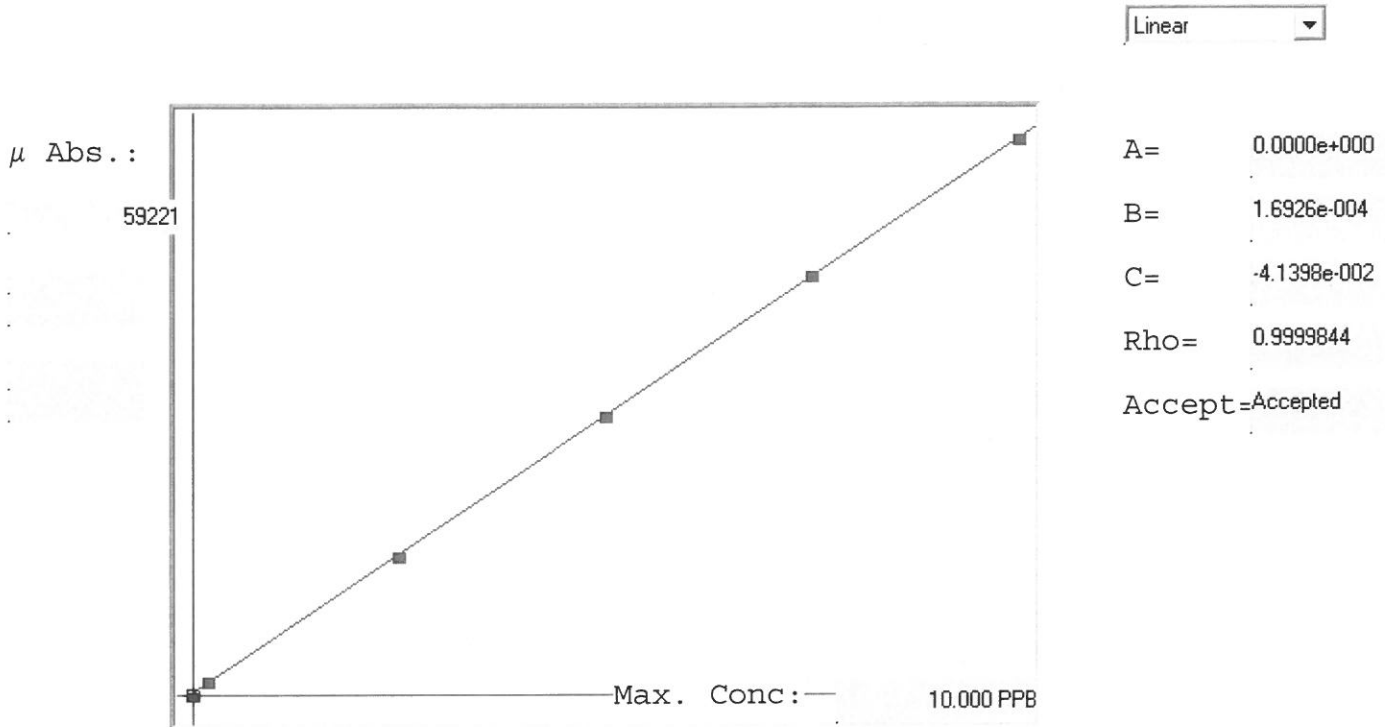

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.011	-0.011	177	0.000	177				
0.2	0.200	0.222	0.022	1556	0.0 %	1556				
2.5	2.500	2.481	-0.019	14900	0.0 %	14900				
5.0	5.000	4.992	-0.008	29740	0.0 %	29740				
7.5	7.500	7.534	0.034	44759	0.0 %	44759				
10.0	10.000	9.982	-0.018	59221	0.0 %	59221				

LB104587 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 14 Aug 2019 10:52:13			
Sample ID	Extended ID	µ Abs.	Conc.	Std CondMethod	Units	Date	Type
0.0 - 1	50-0	177	-	0.00007471B	PPB	14 Aug 2019 11:05:13	S Std
0.2 - 1	50-2	1556	-	0.20007471B	PPB	14 Aug 2019 11:07:31	S Std
2.5 - 1	52-5	14900	-	2.50007471B	PPB	14 Aug 2019 11:09:50	S Std
5.0 - 1	55-0	29740	-	5.00007471B	PPB	14 Aug 2019 11:12:08	S Std
7.5 - 1	57-5	44759	-	7.50007471B	PPB	14 Aug 2019 11:14:25	S Std
10.0 - 1	510-0	59221	-	10.00007471B	PPB	14 Aug 2019 11:16:42	S Std
ICV69 - 1	ICV69	22998	3.8512	-7471B	PPB	14 Aug 2019 11:21:32	U SMPL
ICB69 - 1	ICB69	315	0.0119	-7471B	PPB	14 Aug 2019 11:23:47	U SMPL
CCV12 - 1	CCV12	29677	4.9817	-7471B	PPB	14 Aug 2019 11:26:04	U SMPL
CCB12 - 1	CCB12	257	0.0021	-7471B	PPB	14 Aug 2019 11:28:20	U SMPL
CRA - 1	CRA	1500	0.2125	-7471B	PPB	14 Aug 2019 11:30:36	U SMPL
HighStd - 1	HighStd	59267	9.9900	-7471B	PPB	14 Aug 2019 11:32:52	U SMPL
ChkStd - 1	ChkStd	41434	6.9716	-7471B	PPB	14 Aug 2019 11:35:09	U SMPL
PB122264BL - 1	PBS	-30	-0.0465	-7471B	PPB	14 Aug 2019 11:37:26	U SMPL
PB122264BS - 1	LCSS	21977	3.6784	-7471B	PPB	14 Aug 2019 11:39:44	U SMPL
K4085-01 - 1	HR-05-080919-A	3501	0.5512	-7471B	PPB	14 Aug 2019 11:42:01	U SMPL
K4085-01DUP - 1	HR-05-080919-ADUP	3476	0.5469	-7471B	PPB	14 Aug 2019 11:44:18	U SMPL
K4085-01MS - 1	HR-05-080919-AMS	24794	4.1552	-7471B	PPB	14 Aug 2019 11:46:36	U SMPL
K4085-01MSD - 1	HR-05-080919-AMSD	26035	4.3652	-7471B	PPB	14 Aug 2019 11:48:54	U SMPL
K4085-03 - 1	HR-05-080919-B	2266	0.3421	-7471B	PPB	14 Aug 2019 11:51:10	U SMPL
CCV13 - 1	CCV13	29761	4.9959	-7471B	PPB	14 Aug 2019 11:53:26	U SMPL
CCB13 - 1	CCB13	278	0.0057	-7471B	PPB	14 Aug 2019 11:55:42	U SMPL
K4085-05 - 1	HR-05-080919-C	1370	0.1905	-7471B	PPB	14 Aug 2019 11:58:00	U SMPL
K4090-05 - 1	OR-03-080919-A	1562	0.2230	-7471B	PPB	14 Aug 2019 12:00:16	U SMPL
K4090-07 - 1	OR-03-080919-B	1840	0.2700	-7471B	PPB	14 Aug 2019 12:02:32	U SMPL
K4095-05 - 1	SU-04-080919-A	2233	0.3366	-7471B	PPB	14 Aug 2019 12:04:48	U SMPL
K4095-07 - 1	SU-04-080919-B	1979	0.2936	-7471B	PPB	14 Aug 2019 12:07:05	U SMPL
K4236-04 - 1	20190647	3140	0.4901	-7471B	PPB	14 Aug 2019 12:09:21	U SMPL
K4266-01 - 1	R1-R2(A1-A4)-(0-1)	330	0.0145	-7471B	PPB	14 Aug 2019 12:11:39	U SMPL
K4266-11 - 1	R1-R2-C1-C4-(0-1)	207	-0.0064	-7471B	PPB	14 Aug 2019 12:13:56	U SMPL
K4266-16 - 1	R1-R2-C1-C4-(4.3)	255	0.0018	-7471B	PPB	14 Aug 2019 12:16:14	U SMPL
K4277-01 - 1	TP-19	75195	12.6859	-7471B	PPB	14 Aug 2019 12:18:30	U SMPL
CCV14 - 1	CCV14	30043	5.0436	-7471B	PPB	14 Aug 2019 12:20:46	U SMPL
CCB14 - 1	CCB14	278	0.0057	-7471B	PPB	14 Aug 2019 12:23:04	U SMPL
K4277-05 - 1	TP-20	14124	2.3492	-7471B	PPB	14 Aug 2019 12:25:21	U SMPL
K4277-09 - 1	TP-22	3182	0.4972	-7471B	PPB	14 Aug 2019 12:27:37	U SMPL
K4292-01 - 1	RO-COMP-WS	50708	8.5413	-7471B	PPB	14 Aug 2019 12:29:53	U SMPL
K4294-01 - 1	RT-3425	517	0.0461	-7471B	PPB	14 Aug 2019 12:32:09	U SMPL
K4294-04 - 1	RT-5124	1561	0.2228	-7471B	PPB	14 Aug 2019 12:34:27	U SMPL
K4294-07 - 1	RBR-200052	984	0.1252	-7471B	PPB	14 Aug 2019 12:36:44	U SMPL
K4294-10 - 1	RT-3860	1977	0.2932	-7471B	PPB	14 Aug 2019 12:39:01	U SMPL
PB122265BL - 1	PBS	307	0.0106	-7471B	PPB	14 Aug 2019 12:41:18	U SMPL
PB122265BS - 1	LCSS	23148	3.8766	-7471B	PPB	14 Aug 2019 12:43:36	U SMPL
K4088-01 - 1	CL-01-081219	6948	1.1346	-7471B	PPB	14 Aug 2019 12:45:53	U SMPL
CCV15 - 1	CCV15	29030	4.8722	-7471B	PPB	14 Aug 2019 12:48:10	U SMPL
CCB15 - 1	CCB15	298	0.0090	-7471B	PPB	14 Aug 2019 12:50:27	U SMPL
K4088-01DUP - 1	CL-01-081219DUP	6993	1.1422	-7471B	PPB	14 Aug 2019 12:52:44	U SMPL
K4088-01MS - 1	CL-01-081219MS	29631	4.9739	-7471B	PPB	14 Aug 2019 12:55:01	U SMPL
K4088-01MSD - 1	CL-01-081219MSD	28762	4.8268	-7471B	PPB	14 Aug 2019 12:57:18	U SMPL
K4089-01 - 1	OK-03-081219	841	0.1009	-7471B	PPB	14 Aug 2019 12:59:36	U SMPL
K4096-01 - 1	TR-04-081219	2109	0.3156	-7471B	PPB	14 Aug 2019 13:01:53	U SMPL
K4319-03 - 1	SOIL-PILE	4356	0.6959	-7471B	PPB	14 Aug 2019 13:04:10	U SMPL
K4319-04 - 1	TRANSFORMER-CONTAINMENT-SOIL	7089	1.1585	-7471B	PPB	14 Aug 2019 13:06:27	U SMPL
K4319-05 - 1	TEST-PIT-1	3192	0.4989	-7471B	PPB	14 Aug 2019 13:08:44	U SMPL
K4319-07 - 1	TEST-PIT-2	4383	0.7005	-7471B	PPB	14 Aug 2019 13:11:02	U SMPL
K4321-01 - 1	SP-1	842	0.1011	-7471B	PPB	14 Aug 2019 13:13:18	U SMPL
CCV16 - 1	CCV16	29117	4.8869	-7471B	PPB	14 Aug 2019 13:15:35	U SMPL
CCB16 - 1	CCB16	296	0.0087	-7471B	PPB	14 Aug 2019 13:17:51	U SMPL
K4321-03 - 1	SP-2	1681	0.2431	-7471B	PPB	14 Aug 2019 13:20:09	U SMPL
K4321-05 - 1	SP-3	4431	0.7086	-7471B	PPB	14 Aug 2019 13:22:26	U SMPL
K4324-01 - 1	T8-F1-(0-4)	20305	3.3954	-7471B	PPB	14 Aug 2019 13:24:42	U SMPL
K4324-04 - 1	T8-E1-(0-4)	20116	3.3634	-7471B	PPB	14 Aug 2019 13:26:58	U SMPL
K4324-07 - 1	T8-C1-(0-4)	13542	2.2507	-7471B	PPB	14 Aug 2019 13:29:15	U SMPL
K4328-01 - 1	20190612-LOC-15-CF	335	0.0153	-7471B	PPB	14 Aug 2019 13:31:32	U SMPL
K4085-01LX5 - 1		791	0.0925	-7471B	PPB	14 Aug 2019 13:33:50	U SMPL
K4085-01A - 1		25423	4.2616	-7471B	PPB	14 Aug 2019 13:36:07	U SMPL
K4088-01LX5 - 1		1392	0.1942	-7471B	PPB	14 Aug 2019 13:38:25	U SMPL
K4088-01A - 1		29240	4.9077	-7471B	PPB	14 Aug 2019 13:40:41	U SMPL
CCV17 - 1	CCV17	29057	4.8767	-7471B	PPB	14 Aug 2019 13:42:59	U SMPL
CCB17 - 1	CCB17	89	-0.0263	-7471B	PPB	14 Aug 2019 13:45:16	U SMPL
K4277-01DLX3 - 1		25517	4.2775	-7471B	PPB	14 Aug 2019 13:47:33	U SMPL
CCV18 - 1	CCV18	29167	4.8953	-7471B	PPB	14 Aug 2019 13:49:50	U SMPL
CCB18 - 1	CCB18	331	0.0146	-7471B	PPB	14 Aug 2019 13:52:08	U SMPL