


LB104619

7471B

INSTRUMENT ID: CU1

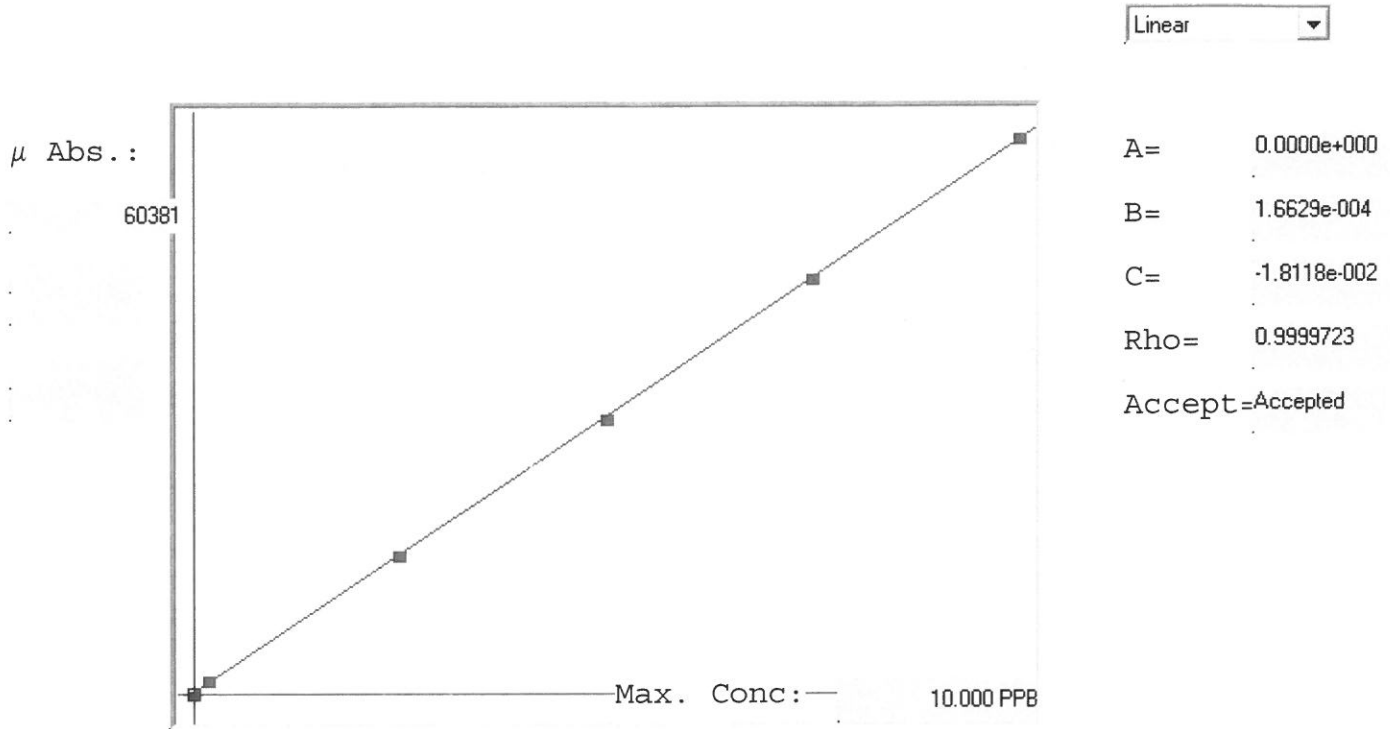

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.010	-0.010	47	0.000	47				
0.2	0.200	0.240	0.040	1555	0.0 %	1555				
2.5	2.500	2.492	-0.008	15095	0.0 %	15095				
5.0	5.000	4.953	-0.047	29895	0.0 %	29895				
7.5	7.500	7.502	0.002	45219	0.0 %	45219				
10.0	10.000	10.023	0.023	60381	0.0 %	60381				

LB104619 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 15 Aug 2019 10:14:27

Sample ID	Extended ID	μ Abs	Conc	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50.0	47	-	0.00007471B	PPB	15 Aug 2019 10:17:07	S	Std
0.2 - 1	50.2	1555	-	0.20007471B	PPB	15 Aug 2019 10:19:26	S	Std
2.5 - 1	52.5	15095	-	2.50007471B	PPB	15 Aug 2019 10:21:44	S	Std
5.0 - 1	55.0	29895	-	5.00007471B	PPB	15 Aug 2019 10:24:02	S	Std
7.5 - 1	57.5	45219	-	7.50007471B	PPB	15 Aug 2019 10:26:19	S	Std
10.0 - 1	510.0	60381	-	10.00007471B	PPB	15 Aug 2019 10:28:37	S	Std
ICV71 - 1	ICV71	23412	3.8752	-7471B	PPB	15 Aug 2019 10:31:28	U	SMPL
ICB71 - 1	ICB71	-25	-0.0223	-7471B	PPB	15 Aug 2019 10:33:44	U	SMPL
CCV22 - 1	CCV22	29674	4.9165	-7471B	PPB	15 Aug 2019 10:36:00	U	SMPL
CCB22 - 1	CCB22	-30	-0.0231	-7471B	PPB	15 Aug 2019 10:38:15	U	SMPL
CRA - 1	CRA	1577	0.2441	-7471B	PPB	15 Aug 2019 10:40:32	U	SMPL
HighStd - 1	HighStd	59939	9.9494	-7471B	PPB	15 Aug 2019 10:42:48	U	SMPL
ChkStd - 1	ChkStd	41574	6.8954	-7471B	PPB	15 Aug 2019 10:45:04	U	SMPL
PB122296BL - 1	PB122296BL	-51	-0.0266	-7471B	PPB	15 Aug 2019 10:47:21	U	SMPL
PB122296BS - 1	PB122296BS	22567	3.7347	-7471B	PPB	15 Aug 2019 10:49:39	U	SMPL
K4264-21 - 1	REACTOR-3-C1-C4-(3)	7548	1.2371	-7471B	PPB	15 Aug 2019 10:51:56	U	SMPL
K4264-21DUP - 1	REACTOR-3-C1-C4-(3)DUP	7560	1.2391	-7471B	PPB	15 Aug 2019 10:54:13	U	SMPL
K4264-21MS - 1	REACTOR-3-C1-C4-(3)MS	29202	4.8380	-7471B	PPB	15 Aug 2019 10:56:31	U	SMPL
K4264-21MSD - 1	REACTOR-3-C1-C4-(3)MSD	27946	4.6292	-7471B	PPB	15 Aug 2019 10:58:49	U	SMPL
K4265-20 - 1	REACTOR-4-A1-A4-(0-1)	7042	1.1529	-7471B	PPB	15 Aug 2019 11:01:04	U	SMPL
CCV23 - 1	CCV23	29777	4.9336	-7471B	PPB	15 Aug 2019 11:03:20	U	SMPL
CCB23 - 1	CCB23	-60	-0.0281	-7471B	PPB	15 Aug 2019 11:05:36	U	SMPL
K4329-01 - 1	ETGI-292	717167	HIGH	-7471B	PPB	15 Aug 2019 11:07:53	X	
K4330-07 - 1	0632-COMP-C	8402	1.3791	-7471B	PPB	15 Aug 2019 11:09:43	U	SMPL
K4330-08 - 1	0633-COMP-D	8092	1.3275	-7471B	PPB	15 Aug 2019 11:12:02	U	SMPL
K4331-05 - 1	0625-COMP-B	6434	1.0518	-7471B	PPB	15 Aug 2019 11:14:18	U	SMPL
K4332-05 - 1	0619-COMP-A	8353	1.3709	-7471B	PPB	15 Aug 2019 11:16:34	U	SMPL
K4339-01 - 1	T8-A1-A4-(0-4)	55900	9.2778	-7471B	PPB	15 Aug 2019 11:18:51	U	SMPL
K4339-10 - 1	T8-B1-(0-4)	25114	4.1582	-7471B	PPB	15 Aug 2019 11:21:08	U	SMPL
K4340-01 - 1	LS-SAMPLE-1	1172	0.1768	-7471B	PPB	15 Aug 2019 11:23:26	U	SMPL
K4340-03 - 1	LS-SAMPLE-2	324	0.0358	-7471B	PPB	15 Aug 2019 11:25:45	U	SMPL
K4355-01 - 1	RBR-200057-200054	3567	0.5751	-7471B	PPB	15 Aug 2019 11:28:01	U	SMPL
CCV24 - 1	CCV24	29779	4.9340	-7471B	PPB	15 Aug 2019 11:30:17	U	SMPL
CCB24 - 1	CCB24	-23	-0.0219	-7471B	PPB	15 Aug 2019 11:32:33	U	SMPL
K4356-01 - 1	TP-1	456	0.0577	-7471B	PPB	15 Aug 2019 11:34:49	U	SMPL
K4356-03 - 1	TP-2	199	0.0150	-7471B	PPB	15 Aug 2019 11:37:05	U	SMPL
K4356-05 - 1	TP-3	1449	0.2228	-7471B	PPB	15 Aug 2019 11:39:21	U	SMPL
K4356-07 - 1	TP-4	780	0.1116	-7471B	PPB	15 Aug 2019 11:41:38	U	SMPL
K4356-09 - 1	TP-5	5670	0.9248	-7471B	PPB	15 Aug 2019 11:43:54	U	SMPL
K4356-11 - 1	TP-6	15756	2.6020	-7471B	PPB	15 Aug 2019 11:46:11	U	SMPL
K4356-13 - 1	TP-7	2127	0.3356	-7471B	PPB	15 Aug 2019 11:48:28	U	SMPL
K4264-21LX5 - 1		1450	0.2230	-7471B	PPB	15 Aug 2019 11:50:45	U	SMPL
K4264-21A - 1		29123	4.8249	-7471B	PPB	15 Aug 2019 11:53:03	U	SMPL
K4329-01DLX10 - 1		141303	23.4798	-7471B	PPB	15 Aug 2019 11:55:19	U	SMPL
CCV25 - 1	CCV25	29889	4.9523	-7471B	PPB	15 Aug 2019 11:57:35	U	SMPL
CCB25 - 1	CCB25	-21	-0.0216	-7471B	PPB	15 Aug 2019 11:59:54	U	SMPL
K4329-01DL2X50 - 1		28336	4.6940	-7471B	PPB	15 Aug 2019 12:02:11	U	SMPL
CCV26 - 1	CCV26	29912	4.9561	-7471B	PPB	15 Aug 2019 12:04:27	U	SMPL
CCB26 - 1	CCB26	-23	-0.0219	-7471B	PPB	15 Aug 2019 12:06:43	U	SMPL