


LB104632

7470A

INSTRUMENT ID : CV1

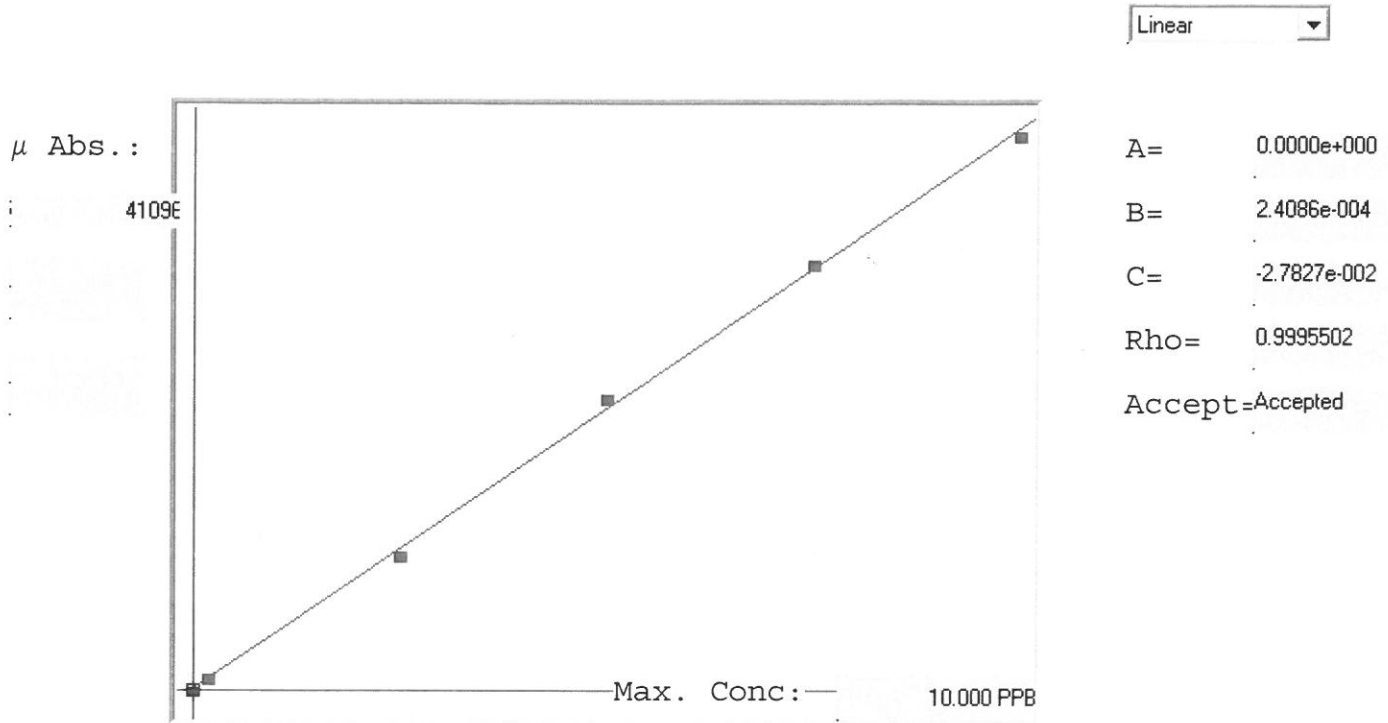

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.012	-0.012	67	0.000	67				
0.2	0.200	0.199	-0.001	941	0.0 %	941				
2.5	2.500	2.376	-0.124	9980	0.0 %	9980				
5.0	5.000	5.187	0.187	21649	0.0 %	21649				
7.5	7.500	7.580	0.080	31586	0.0 %	31586				
10.0	10.000	9.870	-0.130	41096	0.0 %	41096				

LB104632 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 15 Aug 2019 14:09:20

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	67	-	0.0000	7470A	PPB	15 Aug 2019 14:12:18	S	Std
0.2 - 1	50.2	941	-	0.2000	7470A	PPB	15 Aug 2019 14:14:27	S	Std
2.5 - 1	52.5	9980	-	2.5000	7470A	PPB	15 Aug 2019 14:16:36	S	Std
5.0 - 1	55.0	21649	-	5.0000	7470A	PPB	15 Aug 2019 14:18:44	S	Std
7.5 - 1	57.5	31586	-	7.5000	7470A	PPB	15 Aug 2019 14:20:52	S	Std
10.0 - 1	510.0	41096	-	10.0000	7470A	PPB	15 Aug 2019 14:31:00	S	Std
ICV72 - 1	ICV72	16138	3.8591	-7470A	PPB	15 Aug 2019 14:33:34	U	SMPL	
ICB72 - 1	ICB72	-14	-0.0312	-7470A	PPB	15 Aug 2019 14:35:41	U	SMPL	
CCV27 - 1	CCV27	21504	5.1516	-7470A	PPB	15 Aug 2019 14:37:48	U	SMPL	
CCB27 - 1	CCB27	-5	-0.0290	-7470A	PPB	15 Aug 2019 14:39:54	U	SMPL	
CRA - 1	CRA	914	0.1923	-7470A	PPB	15 Aug 2019 14:42:01	U	SMPL	
HighStd - 1	HighStd	41321	9.9247	-7470A	PPB	15 Aug 2019 14:44:07	U	SMPL	
ChkStd - 1	ChkStd	28738	6.8940	-7470A	PPB	15 Aug 2019 14:46:14	U	SMPL	
PB122309BL - 1	PBW	-7	-0.0295	-7470A	PPB	15 Aug 2019 14:48:22	U	SMPL	
PB122309BS - 1	LCSW	16322	3.9035	-7470A	PPB	15 Aug 2019 14:50:29	U	SMPL	
K4324-10 - 1	T8-F1-(0-4)	23	-0.0223	-7470A	PPB	15 Aug 2019 14:52:36	U	SMPL	
K4324-10DUP - 1	T8-F1-(0-4)DUP	36	-0.0192	-7470A	PPB	15 Aug 2019 14:54:44	U	SMPL	
K4324-10MS - 1	T8-F1-(0-4)MS	17086	4.0875	-7470A	PPB	15 Aug 2019 14:56:52	U	SMPL	
K4324-10MSD - 1	T8-F1-(0-4)MSD	17071	4.0839	-7470A	PPB	15 Aug 2019 14:59:01	U	SMPL	
K4324-13 - 1	T8-E1-(0-4)	6	-0.0264	-7470A	PPB	15 Aug 2019 15:01:08	U	SMPL	
CCV28 - 1	CCV28	21291	5.1003	-7470A	PPB	15 Aug 2019 15:03:14	U	SMPL	
CCB28 - 1	CCB28	4	-0.0269	-7470A	PPB	15 Aug 2019 15:05:21	U	SMPL	
K4324-16 - 1	T8-C1-(0-4)	66	-0.0119	-7470A	PPB	15 Aug 2019 15:07:28	U	SMPL	
K4325-02 - 1	20190612-LOC-14	69	-0.0112	-7470A	PPB	15 Aug 2019 15:09:35	U	SMPL	
K4329-02 - 1	ETGI-292	146	0.0073	-7470A	PPB	15 Aug 2019 15:11:42	U	SMPL	
K4339-13 - 1	T8-A1-A4-(0-4)	36	-0.0192	-7470A	PPB	15 Aug 2019 15:13:49	U	SMPL	
K4339-22 - 1	T8-B1-(0-4)	79	-0.0088	-7470A	PPB	15 Aug 2019 15:15:56	U	SMPL	
K4340-02 - 1	LS-SAMPLE-1	36	-0.0192	-7470A	PPB	15 Aug 2019 15:18:04	U	SMPL	
K4340-04 - 1	LS-SAMPLE-2	44	-0.0172	-7470A	PPB	15 Aug 2019 15:20:12	U	SMPL	
PB122312BL - 1	PBW	57	-0.0141	-7470A	PPB	15 Aug 2019 15:22:20	U	SMPL	
PB122312BS - 1	LCSW	16402	3.9227	-7470A	PPB	15 Aug 2019 15:24:29	U	SMPL	
K4329-04 - 1	WATER-PIT	69	-0.0112	-7470A	PPB	15 Aug 2019 15:26:36	U	SMPL	
CCV29 - 1	CCV29	21014	5.0336	-7470A	PPB	15 Aug 2019 15:28:43	U	SMPL	
CCB29 - 1	CCB29	9	-0.0257	-7470A	PPB	15 Aug 2019 15:30:50	U	SMPL	
K4329-04DUP - 1	WATER-PITDUP	74	-0.0100	-7470A	PPB	15 Aug 2019 15:32:56	U	SMPL	
K4329-04MS - 1	WATER-PITMS	16402	3.9227	-7470A	PPB	15 Aug 2019 15:35:03	U	SMPL	
K4329-04MSD - 1	WATER-PITMSD	16557	3.9601	-7470A	PPB	15 Aug 2019 15:37:09	U	SMPL	
K4333-02 - 1	FRAC-TANK	11	-0.0252	-7470A	PPB	15 Aug 2019 15:39:17	U	SMPL	
PB122309TB - 1	PB122242TB	47	-0.0165	-7470A	PPB	15 Aug 2019 15:41:25	U	SMPL	
PB122312TB - 1	PB122244TB	42	-0.0177	-7470A	PPB	15 Aug 2019 15:43:32	U	SMPL	
K4324-10LX5 - 1		20	-0.0230	-7470A	PPB	15 Aug 2019 15:45:40	U	SMPL	
K4324-10A - 1		16908	4.0446	-7470A	PPB	15 Aug 2019 15:47:48	U	SMPL	
K4329-04LX5 - 1		9	-0.0257	-7470A	PPB	15 Aug 2019 15:49:57	U	SMPL	
K4329-04A - 1		16432	3.9300	-7470A	PPB	15 Aug 2019 15:52:04	U	SMPL	
CCV30 - 1	CCV30	20412	4.8886	-7470A	PPB	15 Aug 2019 15:54:11	U	SMPL	
CCB30 - 1	CCB30	104	-0.0028	-7470A	PPB	15 Aug 2019 15:59:20	U	SMPL	