


LB104652

7470A

INSTRUMENT ID: CU1

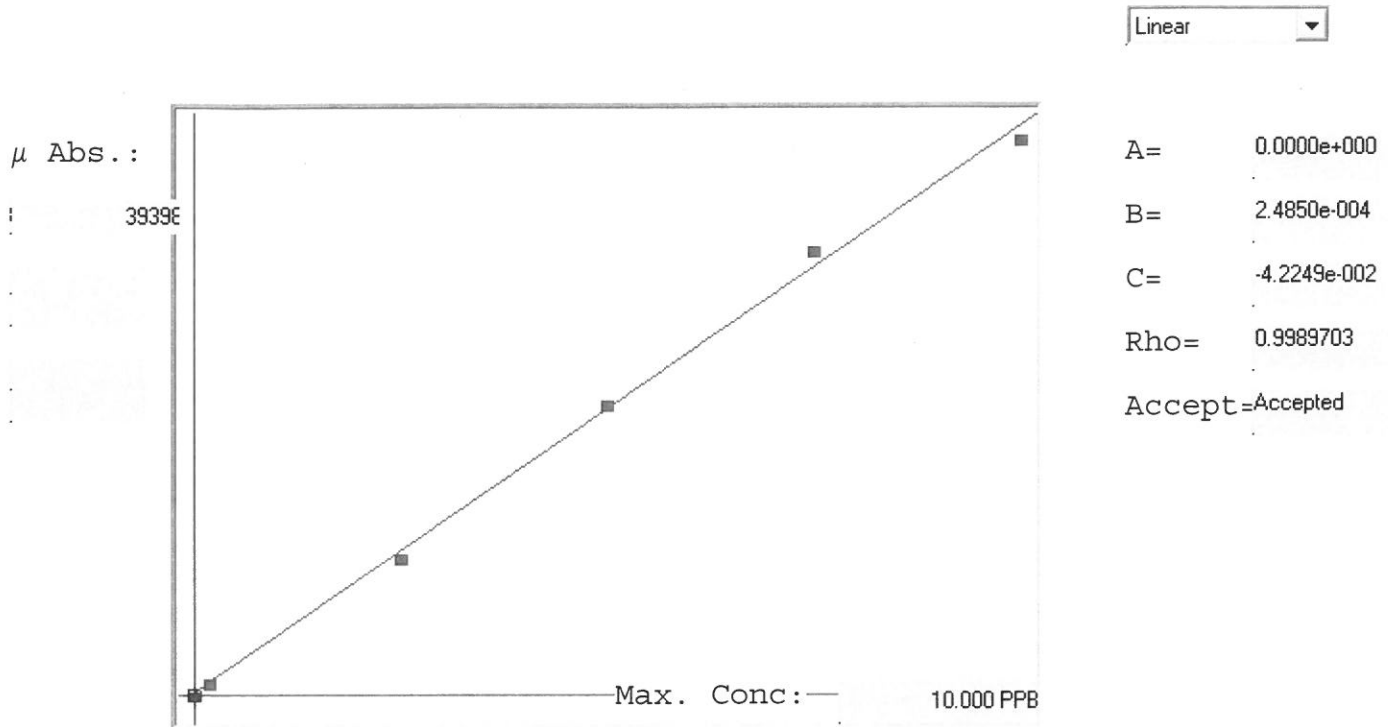

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.011	-0.011	124	0.000	124				
0.2	0.200	0.193	-0.007	946	0.0 %	946				
2.5	2.500	2.385	-0.115	9766	0.0 %	9766				
5.0	5.000	5.101	0.101	20699	0.0 %	20699				
7.5	7.500	7.784	0.284	31496	0.0 %	31496				
10.0	10.000	9.748	-0.252	39398	0.0 %	39398				

LB104652 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 16 Aug 2019 12:40:53				
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
0.0 - 1	50-0	124	-	0.0000	7470A	PPB	16 Aug 2019 12:53:40	S Std
0.2 - 1	50-2	946	-	0.2000	7470A	PPB	16 Aug 2019 12:55:50	S Std
2.5 - 1	52-5	9766	-	2.5000	7470A	PPB	16 Aug 2019 12:57:59	S Std
5.0 - 1	55-0	20699	-	5.0000	7470A	PPB	16 Aug 2019 13:00:07	S Std
7.5 - 1	55-0	31496	-	7.5000	7470A	PPB	16 Aug 2019 13:02:15	S Std
10.0 - 1	57-5	39398	-	10.0000	7470A	PPB	16 Aug 2019 13:06:50	S Std
ICV73 - 1	ICV73	16173	3.9767	-	7470A	PPB	16 Aug 2019 13:09:21	U SMPL
ICB73 - 1	ICB73	27	-0.0355	-	7470A	PPB	16 Aug 2019 13:11:28	U SMPL
CCV31 - 1	CCV31	20172	4.9705	-	7470A	PPB	16 Aug 2019 13:13:34	U SMPL
CCB31 - 1	CCB31	32	-0.0343	-	7470A	PPB	16 Aug 2019 13:15:40	U SMPL
CRA - 1	CRA	869	0.1737	-	7470A	PPB	16 Aug 2019 13:17:47	U SMPL
HighStd - 1	HighStd	39155	9.6877	-	7470A	PPB	16 Aug 2019 13:19:53	U SMPL
ChkStd - 1	ChkStd	27754	6.8546	-	7470A	PPB	16 Aug 2019 13:22:00	U SMPL
PB122339BL - 1	PBW	-19	-0.0470	-	7470A	PPB	16 Aug 2019 13:24:08	U SMPL
PB122339BS - 1	LCSW	15966	3.9253	-	7470A	PPB	16 Aug 2019 13:26:16	U SMPL
K4277-13 - 1	TP-22	8429	2.0523	-	7470A	PPB	16 Aug 2019 13:28:24	U SMPL
K4277-13DUP - 1	TP-22DUP	8852	2.1575	-	7470A	PPB	16 Aug 2019 13:30:32	U SMPL
K4329-03 - 1	WATER-PIT	8780	2.1396	-	7470A	PPB	16 Aug 2019 13:36:55	U SMPL
CCV32 - 1	CCV32	20813	5.1298	-	7470A	PPB	16 Aug 2019 13:39:03	U SMPL
CCB32 - 1	CCB32	64	-0.0263	-	7470A	PPB	16 Aug 2019 13:41:09	U SMPL
K4333-01 - 1	FRAC-TANK	153	-0.0042	-	7470A	PPB	16 Aug 2019 13:43:16	U SMPL
PB122340BL - 1	PBW	74	-0.0239	-	7470A	PPB	16 Aug 2019 13:45:23	U SMPL
PB122340BS - 1	LCSW	15613	3.8376	-	7470A	PPB	16 Aug 2019 13:47:29	U SMPL
K4264-01 - 1	REACTOR-3-C1-C4-(0-2)	47	-0.0306	-	7470A	PPB	16 Aug 2019 13:49:36	U SMPL
K4264-01DUP - 1	REACTOR-3-C1-C4-(0-2)DUP	74	-0.0239	-	7470A	PPB	16 Aug 2019 13:51:44	U SMPL
K4264-01MS - 1	REACTOR-3-C1-C4-(0-2)MS	16869	4.1497	-	7470A	PPB	16 Aug 2019 13:53:51	U SMPL
K4264-01MSD - 1	REACTOR-3-C1-C4-(0-2)MSD	16396	4.0321	-	7470A	PPB	16 Aug 2019 13:55:59	U SMPL
K4264-06 - 1	REACTOR-3-C1-C4-(3)	22	-0.0368	-	7470A	PPB	16 Aug 2019 13:58:08	U SMPL
K4264-11 - 1	REACTOR-3-G1-G4-(0-2)	56	-0.0283	-	7470A	PPB	16 Aug 2019 14:00:17	U SMPL
K4264-16 - 1	REACTOR-3-G1-G4-(3)	49	-0.0301	-	7470A	PPB	16 Aug 2019 14:02:23	U SMPL
CCV33 - 1	CCV33	20617	5.0811	-	7470A	PPB	16 Aug 2019 14:04:30	U SMPL
CCB33 - 1	CCB33	44	-0.0313	-	7470A	PPB	16 Aug 2019 14:06:36	U SMPL
K4265-01 - 1	REACTOR-4-C-(0-3.4)	48	-0.0303	-	7470A	PPB	16 Aug 2019 14:08:43	U SMPL
K4265-04 - 1	REACTOR-4-B-(0-3.4)	44	-0.0313	-	7470A	PPB	16 Aug 2019 14:10:50	U SMPL
K4265-07 - 1	REACTOR-4-A1-A4-(0-1)	42	-0.0318	-	7470A	PPB	16 Aug 2019 14:12:56	U SMPL
K4265-12 - 1	REACTOR-4-A1-A4-(3.4)	66	-0.0258	-	7470A	PPB	16 Aug 2019 14:15:03	U SMPL
K4265-17 - 1	R1-R2-(0-4.3)	60	-0.0273	-	7470A	PPB	16 Aug 2019 14:17:10	U SMPL
K4272-01 - 1	2S-G1-G4-(0-1)	54	-0.0288	-	7470A	PPB	16 Aug 2019 14:19:18	U SMPL
K4272-06 - 1	2S-G1-G4-(1)	75	-0.0236	-	7470A	PPB	16 Aug 2019 14:21:26	U SMPL
K4272-11 - 1	2S-K-(0-1)	57	-0.0281	-	7470A	PPB	16 Aug 2019 14:23:33	U SMPL
K4356-02 - 1	TP-1	42	-0.0318	-	7470A	PPB	16 Aug 2019 14:25:42	U SMPL
K4356-04 - 1	TP-2	134	-0.0089	-	7470A	PPB	16 Aug 2019 14:27:49	U SMPL
CCV34 - 1	CCV34	20161	4.9677	-	7470A	PPB	16 Aug 2019 14:29:56	U SMPL
CCB34 - 1	CCB34	60	-0.0273	-	7470A	PPB	16 Aug 2019 14:32:03	U SMPL
K4356-06 - 1	TP-3	90	-0.0199	-	7470A	PPB	16 Aug 2019 14:34:10	U SMPL
K4356-08 - 1	TP-4	87	-0.0206	-	7470A	PPB	16 Aug 2019 14:36:19	U SMPL
K4356-10 - 1	TP-5	119	-0.0127	-	7470A	PPB	16 Aug 2019 14:38:26	U SMPL
K4356-12 - 1	TP-6	95	-0.0186	-	7470A	PPB	16 Aug 2019 14:40:33	U SMPL
K4356-14 - 1	TP-7	94	-0.0189	-	7470A	PPB	16 Aug 2019 14:42:41	U SMPL
PB122341BL - 1	PBW	73	-0.0241	-	7470A	PPB	16 Aug 2019 14:44:48	U SMPL
PB122341BS - 1	LCSW	15991	3.9315	-	7470A	PPB	16 Aug 2019 14:46:56	U SMPL
K3616-07 - 1	JC-03-081519-A	523	0.0877	-	7470A	PPB	16 Aug 2019 14:49:05	U SMPL
K3616-07MS - 1	JC-03-081519-AMS	16901	4.1576	-	7470A	PPB	16 Aug 2019 14:53:21	U SMPL
CCV35 - 1	CCV35	20553	5.0651	-	7470A	PPB	16 Aug 2019 14:55:28	U SMPL
CCB35 - 1	CCB35	82	-0.0219	-	7470A	PPB	16 Aug 2019 14:57:35	U SMPL
K3616-07MSD - 1	JC-03-081519-AMSD	16123	3.9643	-	7470A	PPB	16 Aug 2019 14:59:42	U SMPL
K3616-14 - 1	JC-03-081519-B	19	-0.0375	-	7470A	PPB	16 Aug 2019 15:01:49	U SMPL
K3616-17 - 1	JC-03-081519-C	303	0.0330	-	7470A	PPB	16 Aug 2019 15:03:56	U SMPL
K4090-12 - 1	OR-02-081519	370	0.0497	-	7470A	PPB	16 Aug 2019 15:06:03	U SMPL
K4371-01 - 1	VNJ-222	845	0.1677	-	7470A	PPB	16 Aug 2019 15:08:11	U SMPL
K4372-02 - 1	SOIL-COMPOSITE	1090	0.2286	-	7470A	PPB	16 Aug 2019 15:10:19	U SMPL
K4377-02 - 1	RBR-50	720	0.1367	-	7470A	PPB	16 Aug 2019 15:12:27	U SMPL
K4377-04 - 1	RBR-29	86	-0.0209	-	7470A	PPB	16 Aug 2019 15:14:35	U SMPL
PB122340TB - 1	PB122275TB	124	-0.0114	-	7470A	PPB	16 Aug 2019 15:16:44	U SMPL
PB122341TB - 1	PB122314TB	262	0.0229	-	7470A	PPB	16 Aug 2019 15:18:52	U SMPL
CCV36 - 1	CCV36	20464	5.0430	-	7470A	PPB	16 Aug 2019 15:21:00	U SMPL
CCB36 - 1	CCB36	47	-0.0306	-	7470A	PPB	16 Aug 2019 15:23:07	U SMPL
K4277-13LX5 - 1		1687	0.3770	-	7470A	PPB	16 Aug 2019 15:25:15	U SMPL
K4264-01LX5 - 1		-17	-0.0465	-	7470A	PPB	16 Aug 2019 15:29:30	U SMPL
K4264-01A - 1		16899	4.1571	-	7470A	PPB	16 Aug 2019 15:31:38	U SMPL
K3616-07LX5 - 1		148	-0.0055	-	7470A	PPB	16 Aug 2019 15:33:46	U SMPL
K3616-07A - 1		16735	4.1164	-	7470A	PPB	16 Aug 2019 15:35:54	U SMPL
K4277-13MS - 1	TP-22MS	25829	6.3762	-	7470A	PPB	16 Aug 2019 15:38:02	U SMPL
K4277-13MSD - 1	TP-22MSD	24615	6.0746	-	7470A	PPB	16 Aug 2019 15:40:10	U SMPL
K4277-13A - K4277-13A		25599	6.3191	-	7470A	PPB	16 Aug 2019 15:42:19	U SMPL
K3616-07 - dup	JC-03-081519ADUP	525	0.0882	-	7470A	PPB	16 Aug 2019 15:44:26	U SMPL
CCV37 - 1	CCV37	20587	5.0736	-	7470A	PPB	16 Aug 2019 15:46:33	U SMPL
CCB37 - 1	CCB37	36	-0.0333	-	7470A	PPB	16 Aug 2019 15:48:41	U SMPL

rs 08-16-19