


LB104661

7471B

INSTRUMENT ID : CU1

Linear

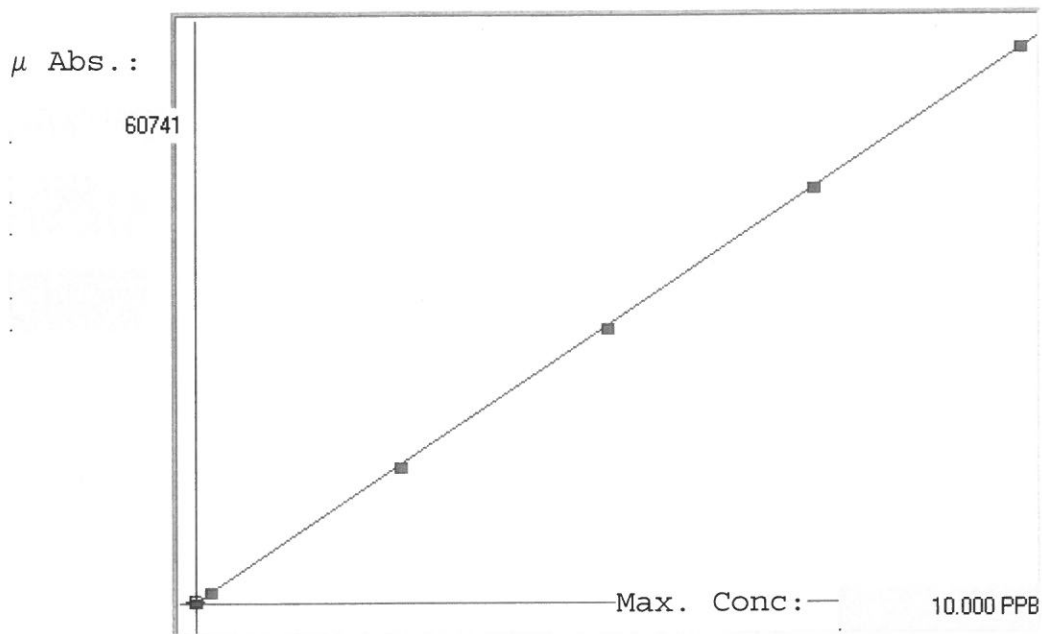

A= 0.0000e+000

B= 1.6521e-004

C= -6.5049e-003

Rho= 0.9999746

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.032	0.032	234	0.000	234				
0.2	0.200	0.209	0.009	1302	0.0 %	1302				
2.5	2.500	2.474	-0.026	15014	0.0 %	15014				
5.0	5.000	4.961	-0.039	30066	0.0 %	30066				
7.5	7.500	7.496	-0.004	45414	0.0 %	45414				
10.0	10.000	10.028	0.028	60741	0.0 %	60741				

LB104661 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 16 Aug 2019 16:42:40

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	234	-	0.00007471B	PPB		16 Aug 2019 16:46:46	S	Std
0.2 - 1	50.2	1302	-	0.20007471B	PPB		16 Aug 2019 16:49:04	S	Std
2.5 - 1	52.5	15014	-	2.50007471B	PPB		16 Aug 2019 16:51:22	S	Std
5.0 - 1	55.0	30066	-	5.00007471B	PPB		16 Aug 2019 16:53:39	S	Std
7.5 - 1	57.5	45414	-	7.50007471B	PPB		16 Aug 2019 16:55:57	S	Std
10.0 - 1	50.0	60741	-	10.00007471B	PPB		16 Aug 2019 16:58:14	S	Std
ICV74 - 1	ICV74	23915	3.9445	-7471B	PPB		16 Aug 2019 17:02:19	U	SMPL
ICB74 - 1	ICB74	98	0.0097	-7471B	PPB		16 Aug 2019 17:04:34	U	SMPL
CCV38 - 1	CCV38	30015	4.9522	-7471B	PPB		16 Aug 2019 17:06:51	U	SMPL
CCB38 - 1	CCB38	97	0.0095	-7471B	PPB		16 Aug 2019 17:09:06	U	SMPL
CRA - 1	CRA	1308	0.2096	-7471B	PPB		16 Aug 2019 17:11:23	U	SMPL
HighStd - 1	HighStd	60367	9.9666	-7471B	PPB		16 Aug 2019 17:13:40	U	SMPL
ChkStd - 1	ChkStd	41809	6.9007	-7471B	PPB		16 Aug 2019 17:15:56	U	SMPL
PB122347BL - 1	PBS	51	0.0019	-7471B	PPB		16 Aug 2019 17:18:13	U	SMPL
PB122347BS - 1	LCSS	20081	3.3110	-7471B	PPB		16 Aug 2019 17:20:31	U	SMPL
K3616-01 - 1	JC-03-081519-A	6416	1.0535	-7471B	PPB		16 Aug 2019 17:22:48	U	SMPL
K3616-08 - 1	JC-03-081519-B	3292	0.5374	-7471B	PPB		16 Aug 2019 17:25:06	U	SMPL
K3616-15 - 1	JC-03-081519-C	7731	1.2707	-7471B	PPB		16 Aug 2019 17:27:24	U	SMPL
K4090-09 - 1	OR-02-081519	2169	0.3518	-7471B	PPB		16 Aug 2019 17:29:42	U	SMPL
K4140-21 - 1	P001-SS008-1824-02	1532	0.2466	-7471B	PPB		16 Aug 2019 17:31:58	U	SMPL
CCV39 - 1	CCV39	29996	4.9491	-7471B	PPB		16 Aug 2019 17:34:15	U	SMPL
CCB39 - 1	CCB39	68	0.0047	-7471B	PPB		16 Aug 2019 17:36:33	U	SMPL
K4140-21DUP - 1	P001-SS008-1824-02DUP	1561	0.2514	-7471B	PPB		16 Aug 2019 17:38:49	U	SMPL
K4140-24 - 1	P001-TP2-1824-02	15913	2.6225	-7471B	PPB		16 Aug 2019 17:41:05	U	SMPL
K4140-24DUP - 1	P001-TP2-1824-02DUP	16011	2.6386	-7471B	PPB		16 Aug 2019 17:43:22	U	SMPL
K4140-41 - 1	k4140-21MS	22741	3.7505	-7471B	PPB		16 Aug 2019 17:45:38	U	SMPL
K4140-42 - 1	k4140-21MSD	23849	3.9335	-7471B	PPB		16 Aug 2019 17:47:55	U	SMPL
K4140-43 - 1	k4140-24MS	38944	6.4274	-7471B	PPB		16 Aug 2019 17:50:12	U	SMPL
K4140-44 - 1	k4140-24MSD	38296	6.3203	-7471B	PPB		16 Aug 2019 17:52:30	U	SMPL
K4350-04 - 1	SS-18_081519	16394	2.7019	-7471B	PPB		16 Aug 2019 17:54:48	U	SMPL
K4350-07 - 1	SP-03_081519	7350	1.2078	-7471B	PPB		16 Aug 2019 17:57:07	U	SMPL
K4365-01 - 1	0600-COMP-BH-1	1034	0.1643	-7471B	PPB		16 Aug 2019 17:59:24	U	SMPL
CCV40 - 1	CCV40	30128	4.9709	-7471B	PPB		16 Aug 2019 18:01:40	U	SMPL
CCB40 - 1	CCB40	55	0.0026	-7471B	PPB		16 Aug 2019 18:03:56	U	SMPL
K4365-02 - 1	0601-COMP-BH-2	4333	0.7093	-7471B	PPB		16 Aug 2019 18:06:13	U	SMPL
K4365-03 - 1	0602-COMP-BH-3	13813	2.2755	-7471B	PPB		16 Aug 2019 18:08:31	U	SMPL
K4365-04 - 1	0603-COMP-BH-4	3359	0.5484	-7471B	PPB		16 Aug 2019 18:10:48	U	SMPL
K4365-05 - 1	0604-COMP-BH-6	2997	0.4886	-7471B	PPB		16 Aug 2019 18:13:04	U	SMPL
K4372-01 - 1	SOIL-COMPOSITE	105642	17.4464	-7471B	PPB		16 Aug 2019 18:15:21	U	SMPL
K4377-01 - 1	RBR-50	1800	0.2909	-7471B	PPB		16 Aug 2019 18:17:41	U	SMPL
K4377-03 - 1	RBR-29	1615	0.2603	-7471B	PPB		16 Aug 2019 18:20:07	U	SMPL
K4383-03 - 1	TP-1359	1074	0.1709	-7471B	PPB		16 Aug 2019 18:22:25	U	SMPL
K4140-21LX5 - 1		400	0.0596	-7471B	PPB		16 Aug 2019 18:24:43	U	SMPL
K4140-21A - 1		22628	3.7318	-7471B	PPB		16 Aug 2019 18:26:59	U	SMPL
CCV41 - 1	CCV41	29647	4.8914	-7471B	PPB		16 Aug 2019 18:29:15	U	SMPL
CCB41 - 1	CCB41	0	-0.0065	-7471B	PPB		16 Aug 2019 18:31:33	U	SMPL
K4140-24LX5 - 1		3156	0.5149	-7471B	PPB		16 Aug 2019 18:33:50	U	SMPL
K4140-24A - 1		38597	6.3700	-7471B	PPB		16 Aug 2019 18:36:06	U	SMPL
K4372-01DLX4 - 1		26483	4.3687	-7471B	PPB		16 Aug 2019 18:38:23	U	SMPL
CCV42 - 1	CCV42	30086	4.9640	-7471B	PPB		16 Aug 2019 18:40:41	U	SMPL
CCB42 - 1	CCB42	165	0.0208	-7471B	PPB		16 Aug 2019 18:42:58	U	SMPL