


LB104762

245.1

INSTRUMENT ID : CUI

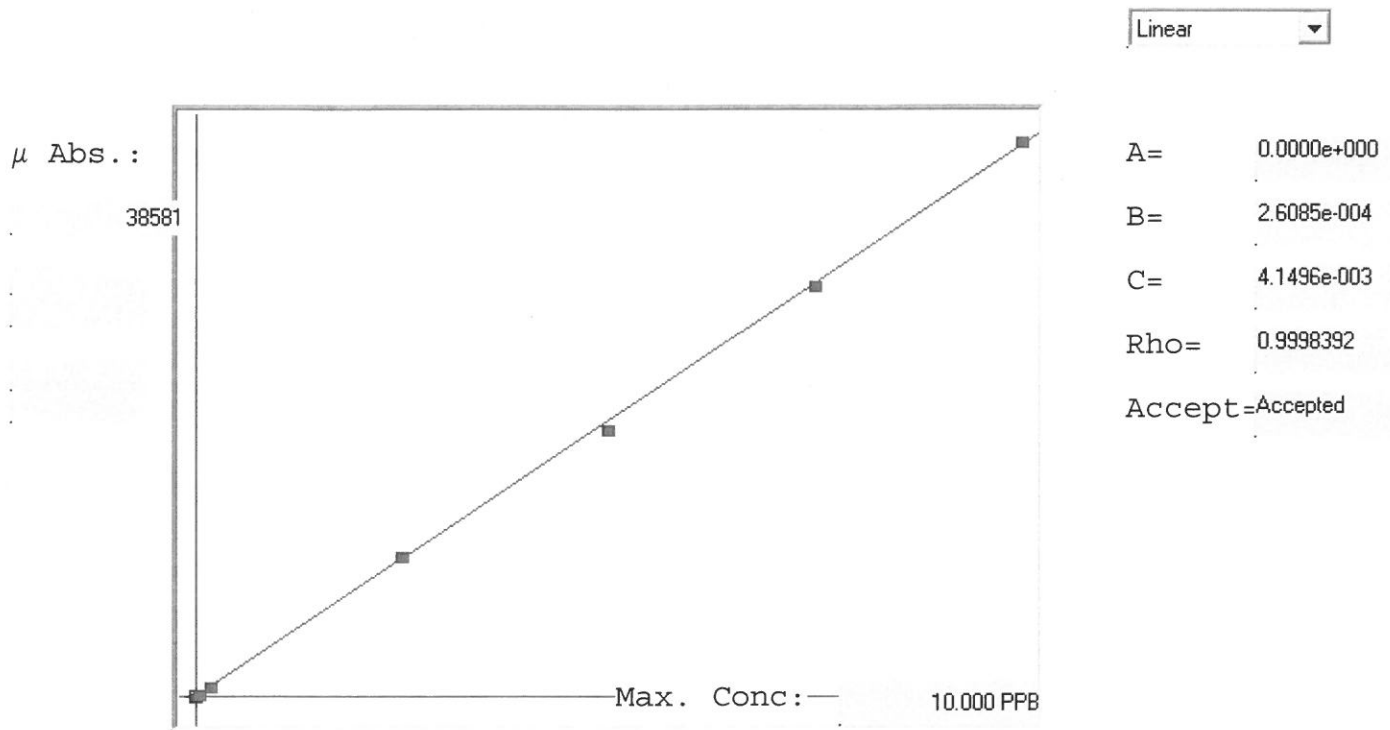

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.032	0.032	105	0.000	105				
0.05	0.050	0.060	0.010	214	0.0 %	214				
0.2	0.200	0.205	0.005	769	0.0 %	769				
2.5	2.500	2.547	0.047	9748	0.0 %	9748				
5.0	5.000	4.848	-0.152	18571	0.0 %	18571				
7.5	7.500	7.490	-0.010	28699	0.0 %	28699				
10.0	10.000	10.068	0.068	38581	0.0 %	38581				

LB104762 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 23 Aug 2019 08:43:43

Sample ID	Extended ID	μ Abs	Conc	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	105	-	0.0000	245.1	PPB	23 Aug 2019 09:34:58	S	Std
0.05 - 1	50.05	214	-	0.0500	245.1	PPB	23 Aug 2019 09:37:17	S	Std
0.2 - 1	50.2	769	-	0.2000	245.1	PPB	23 Aug 2019 09:39:35	S	Std
2.5 - 1	52.5	9748	-	2.5000	245.1	PPB	23 Aug 2019 09:41:53	S	Std
5.0 - 1	55.0	18571	-	5.0000	245.1	PPB	23 Aug 2019 09:44:10	S	Std
7.5 - 1	57.5	28699	-	7.5000	245.1	PPB	23 Aug 2019 09:46:27	S	Std
10.0 - 1	510.0	38581	-	10.0000	245.1	PPB	23 Aug 2019 10:08:20	S	Std
ICV80 - 1	ICV80	14839	3.8749	-245.1		PPB	23 Aug 2019 10:10:56	U	SMPL
ICB80 - 1	ICB80	57	0.0190	-245.1		PPB	23 Aug 2019 10:13:12	U	SMPL
CCV74 - 1	CCV74	18593	4.8542	-245.1		PPB	23 Aug 2019 10:15:28	U	SMPL
CCB74 - 1	CCB74	123	0.0362	-245.1		PPB	23 Aug 2019 10:26:45	U	SMPL
CRA - 1	CRA	199	0.0561	-245.1		PPB	23 Aug 2019 10:34:59	U	SMPL
HighStd - 1	HighStd	37878	9.8847	-245.1		PPB	23 Aug 2019 10:37:14	U	SMPL
ChkStd - 1	ChkStd	26266	6.8557	-245.1		PPB	23 Aug 2019 10:39:30	U	SMPL
PB122493BL - 1	PBW	-47	-0.0081	-245.1		PPB	23 Aug 2019 10:41:48	U	SMPL
PB122493BS - 1	LCSW	15743	4.1107	-245.1		PPB	23 Aug 2019 10:44:05	U	SMPL
K4320-01 - 1	COMP	1051	0.2783	-245.1		PPB	23 Aug 2019 10:46:22	U	SMPL
K4463-01 - 1	P001-FB-082019-01	149	0.0430	-245.1		PPB	23 Aug 2019 10:48:39	U	SMPL
K4463-02 - 1	P001-SW001-08202019-01	148	0.0428	-245.1		PPB	23 Aug 2019 10:50:57	U	SMPL
K4463-03 - 1	P001-SW002-08202019-01	24	0.0104	-245.1		PPB	23 Aug 2019 10:53:15	U	SMPL
K4463-04 - 1	P001-SW003-08202019-01	44	0.0156	-245.1		PPB	23 Aug 2019 10:55:30	U	SMPL
CCV75 - 1	CCV75	18341	4.7884	-245.1		PPB	23 Aug 2019 10:57:46	U	SMPL
CCB75 - 1	CCB75	-43	-0.0071	-245.1		PPB	23 Aug 2019 11:00:03	U	SMPL
K4463-05 - 1	P001-SW004-08202019-01	65	0.0211	-245.1		PPB	23 Aug 2019 11:02:19	U	SMPL
K4463-05DUP - 1	P001-SW004-08202019-01DUP	79	0.0248	-245.1		PPB	23 Aug 2019 11:08:10	U	SMPL
K4463-06 - 1	K4463-05MS	16678	4.3546	-245.1		PPB	23 Aug 2019 11:14:19	U	SMPL
K4463-07 - 1	K4463-05MSD	16006	4.1793	-245.1		PPB	23 Aug 2019 11:16:35	U	SMPL
K4463-08 - 1	P001-SW004-08202019-02	34	0.0130	-245.1		PPB	23 Aug 2019 11:18:51	U	SMPL
K4463-05LX5 - 1		-189	-0.0452	-245.1		PPB	23 Aug 2019 11:29:09	U	SMPL
K4463-05A - 1		16050	4.1908	-245.1		PPB	23 Aug 2019 11:31:26	U	SMPL
CCV76 - 1	CCV76	17831	4.6554	-245.1		PPB	23 Aug 2019 11:33:43	U	SMPL
CCB76 - 1	CCB76	-152	-0.0355	-245.1		PPB	23 Aug 2019 11:36:01	U	SMPL