


LB104796

7471B

INSTRUMENT ID: CV1

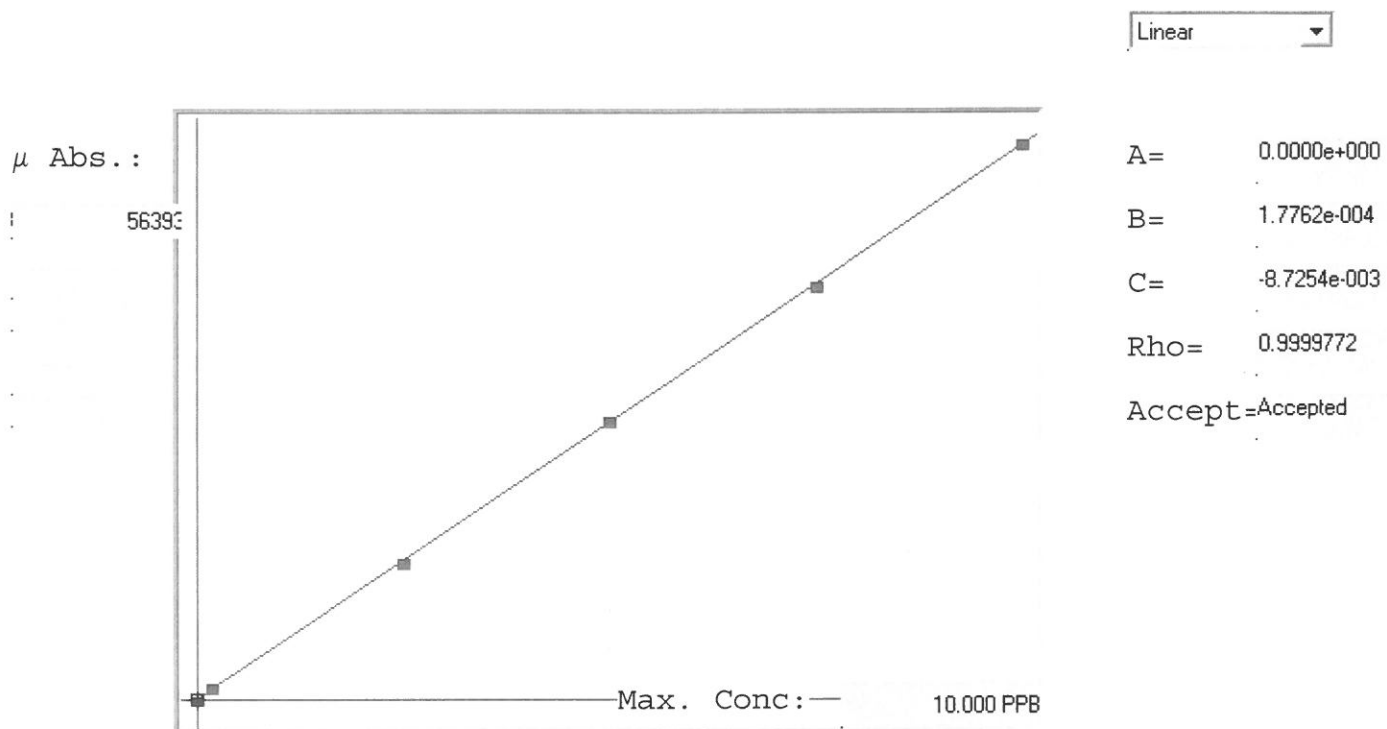

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.002	-0.002	36	0.000	36				
0.2	0.200	0.204	0.004	1195	0.0 %	1195				
2.5	2.500	2.480	-0.020	14013	0.0 %	14013				
5.0	5.000	5.045	0.045	28455	0.0 %	28455				
7.5	7.500	7.465	-0.035	42080	0.0 %	42080				
10.0	10.000	10.008	0.008	56393	0.0 %	56393				

LB104796 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 26 Aug 2019 13:40:58

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50.0	36	-	0.00007471B	PPB	26 Aug 2019 13:42:20	S	Std
0.2 - 1	50.2	1195	-	0.20007471B	PPB	26 Aug 2019 13:44:38	S	Std
2.5 - 1	52.5	14013	-	2.50007471B	PPB	26 Aug 2019 13:46:57	S	Std
5.0 - 1	55.0	28455	-	5.00007471B	PPB	26 Aug 2019 13:49:14	S	Std
7.5 - 1	57.5	42080	-	7.50007471B	PPB	26 Aug 2019 13:51:32	S	Std
10.0 - 1	516.0	56393	-	10.00007471B	PPB	26 Aug 2019 13:53:50	S	Std
ICV83 - 1	ICV83	22387	3.9676	-7471B	PPB	26 Aug 2019 13:56:43	U	SMPL
ICB83 - 1	ICB83	-44	-0.0165	-7471B	PPB	26 Aug 2019 13:59:01	U	SMPL
CCV87 - 1	CCV87	28207	5.0014	-7471B	PPB	26 Aug 2019 14:01:17	U	SMPL
CCB87 - 1	CCB87	-25	-0.0132	-7471B	PPB	26 Aug 2019 14:03:34	U	SMPL
CRA - 1	CRA	1185	0.2018	-7471B	PPB	26 Aug 2019 14:05:50	U	SMPL
HighStd - 1	HighStd	55969	9.9324	-7471B	PPB	26 Aug 2019 14:08:06	U	SMPL
ChkStd - 1	ChkStd	39039	6.9253	-7471B	PPB	26 Aug 2019 14:10:24	U	SMPL
PB122558BL - 1	PB122558BL	-27	-0.0135	-7471B	PPB	26 Aug 2019 14:12:44	U	SMPL
PB122558BS - 1	PB122558BS	19899	3.5257	-7471B	PPB	26 Aug 2019 14:15:02	U	SMPL
K4493-01 - 1	T9-12-13-H-(0-1.9)	969	0.1634	-7471B	PPB	26 Aug 2019 14:17:19	U	SMPL
K4493-01DUP - 1	T9-12-13-H-(0-1.9)DUP	950	0.1600	-7471B	PPB	26 Aug 2019 14:19:37	U	SMPL
K4493-01MS - 1	T9-12-13-H-(0-1.9)MS	23769	4.2131	-7471B	PPB	26 Aug 2019 14:21:54	U	SMPL
K4493-01MSD - 1	T9-12-13-H-(0-1.9)MSD	23144	4.1021	-7471B	PPB	26 Aug 2019 14:24:12	U	SMPL
K4493-04 - 1	T9-12-13-I-(0-1.9)	536	0.0865	-7471B	PPB	26 Aug 2019 14:26:28	U	SMPL
CCV88 - 1	CCV88	28195	4.9992	-7471B	PPB	26 Aug 2019 14:28:45	U	SMPL
CCB88 - 1	CCB88	-25	-0.0132	-7471B	PPB	26 Aug 2019 14:31:01	U	SMPL
K4493-07 - 1	T9-12-13-J-(0-1.9)	569	0.0923	-7471B	PPB	26 Aug 2019 14:33:17	U	SMPL
K4493-10 - 1	T9-12-13-K1-K4-(0-1.9)	7957	1.4046	-7471B	PPB	26 Aug 2019 14:35:33	U	SMPL
K4496-01 - 1	S600-M-1.0-1.5-082219	562	0.0911	-7471B	PPB	26 Aug 2019 14:37:49	U	SMPL
K4496-04 - 1	S600-M-1.0-1.5-082219-FD	511	0.0820	-7471B	PPB	26 Aug 2019 14:40:05	U	SMPL
K4496-11 - 1	S601-M-1.0-1.5-082219	680	0.1121	-7471B	PPB	26 Aug 2019 14:42:22	U	SMPL
K4498-01 - 1	SIDEWALL-1	2340	0.4069	-7471B	PPB	26 Aug 2019 14:44:40	U	SMPL
K4498-02 - 1	SIDEWALL-2	2516	0.4382	-7471B	PPB	26 Aug 2019 14:46:57	U	SMPL
K4498-03 - 1	SIDEWALL-3	4448	0.7813	-7471B	PPB	26 Aug 2019 14:49:14	U	SMPL
K4498-04 - 1	BOTTOM-3	1767	0.3051	-7471B	PPB	26 Aug 2019 14:51:32	U	SMPL
K4498-05 - 1	BOTTOM-4	12448	2.2023	-7471B	PPB	26 Aug 2019 14:53:47	U	SMPL
CCV89 - 1	CCV89	28912	5.1266	-7471B	PPB	26 Aug 2019 14:56:03	U	SMPL
CCB89 - 1	CCB89	-36	-0.0151	-7471B	PPB	26 Aug 2019 14:58:19	U	SMPL
K4499-01 - 1	24408-26706	285836	50.7610	-7471B	PPB	26 Aug 2019 15:00:36	U	SMPL
K4493-01LX5 - 1		-191	-0.0427	-7471B	PPB	26 Aug 2019 15:02:52	U	SMPL
K4493-01A - 1		23590	4.1813	-7471B	PPB	26 Aug 2019 15:05:11	U	SMPL
K4499-01DLX10 - 1		29865	5.2958	-7471B	PPB	26 Aug 2019 15:09:16	U	SMPL
CCV90 - 1	CCV90	29224	5.1820	-7471B	PPB	26 Aug 2019 15:11:32	U	SMPL
CCB90 - 1	CCB90	-32	-0.0144	-7471B	PPB	26 Aug 2019 15:13:49	U	SMPL