

LB104798

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

8/26/2019 14:49

Test: ~~Total~~ ^{Reactive} CN

ug/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.590	0.0	0.083	
ICB1	-0.055	0.0	0.001	
CCV1	248.443	0.0	0.214	
CCB1	-0.261	0.0	0.001	
PB122538BL	-0.308	0.0	0.001	
K4499-02	-0.491	0.0	0.001	
K4499-02DUP	-0.440	0.0	0.001	
K4509-11	-0.579	0.0	0.001	
K4509-12	-0.639	0.0	0.001	
K4509-13	-0.624	0.0	0.001	
K4509-14	-0.418	0.0	0.001	
K4509-15	-0.732	0.0	0.001	
K4510-15	-1.167	0.0	0.000	
K4510-16	-0.365	0.0	0.001	
CCV2	254.595	0.0	0.220	
CCB2	-0.173	0.0	0.001	
K4510-17	-0.432	0.0	0.001	
K4510-18	-0.451	0.0	0.001	
K4510-19	-0.724	0.0	0.001	
K4510-20	-0.556	0.0	0.001	
K4510-21	-0.204	0.0	0.001	
PB122496BL	-0.396	0.0	0.001	
K4090-16DUP	-0.443	0.0	0.001	
K4487-01	-0.418	0.0	0.001	
K4090-16	-0.028	0.0	0.001	
CCV3	265.578	0.0	0.229	
CCB3	-0.293	0.0	0.001	

N	27
Mean	31.593
SD	82.9917
CV%	262.69

8/26/19
CT

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

8/26/2019 13:12


Test ~~Total~~ ^{Reactive} CN

Accepted 8/26/2019 13:11

Factor 1166
Bias 0.001

Coeff. of det. 0.999808

Errors

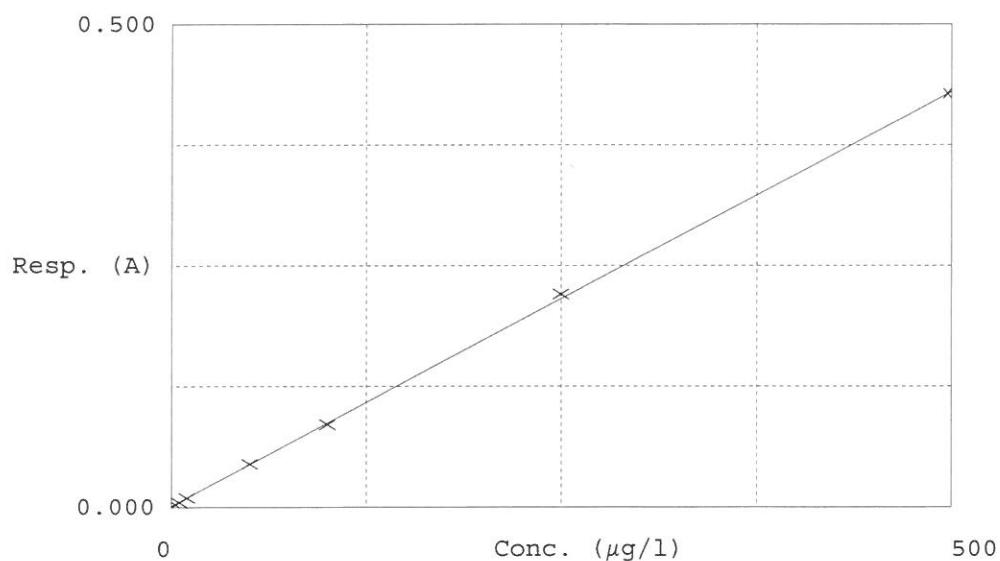

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.7810	0.0000	
2	5.0PPBCN	0.005	4.3182	5.0000	
3	10PPBCN	0.010	9.7647	10.0000	
4	50PPBCN	0.045	50.5268	50.0000	
5	100PPBCN	0.086	98.1507	100.0000	
6	250PPBCN	0.220	255.3840	250.0000	
7	500PPBCN	0.428	497.6367	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Mon Aug 26 12:49:05 2019

Mon Aug 26 14:28:50 2019

MSK

Sample Id	Sam/Ctr/c/	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.781	µg/l	8/26/2019 12:49:05	
5.0PPBCN	A	Reactive CN	P	4.3182	µg/l	8/26/2019 12:49:06	
10PPBCN	A	Reactive CN	P	9.7647	µg/l	8/26/2019 12:49:07	
50PPBCN	A	Reactive CN	P	50.5268	µg/l	8/26/2019 12:49:08	
100PPBCN	A	Reactive CN	P	98.1507	µg/l	8/26/2019 12:49:09	
250PPBCN	A	Reactive CN	P	255.384	µg/l	8/26/2019 12:49:10	
500PPBCN	A	Reactive CN	P	497.6367	µg/l	8/26/2019 12:49:11	
ICV1	S	Reactive CN	P	94.5899	µg/l	8/26/2019 13:50:17	
ICB1	S	Reactive CN	P	-0.0552	µg/l	8/26/2019 13:50:20	
CCV1	S	Reactive CN	P	248.4431	µg/l	8/26/2019 13:50:21	
CCB1	S	Reactive CN	P	-0.2605	µg/l	8/26/2019 13:50:24	
PB122538BL	S	Reactive CN	P	-0.3076	µg/l	8/26/2019 13:50:25	
K4499-02	S	Reactive CN	P	-0.4911	µg/l	8/26/2019 13:50:26	
K4499-02DUP	S	Reactive CN	P	-0.4396	µg/l	8/26/2019 13:50:27	
K4509-11	S	Reactive CN	P	-0.5794	µg/l	8/26/2019 13:57:49	
K4509-12	S	Reactive CN	P	-0.6395	µg/l	8/26/2019 13:57:50	
K4509-13	S	Reactive CN	P	-0.6242	µg/l	8/26/2019 13:57:51	
K4509-14	S	Reactive CN	P	-0.4184	µg/l	8/26/2019 13:57:52	
K4509-15	S	Reactive CN	P	-0.7316	µg/l	8/26/2019 13:57:53	
K4510-15	S	Reactive CN	P	-1.1668	µg/l	8/26/2019 13:57:54	
K4510-16	S	Reactive CN	P	-0.3653	µg/l	8/26/2019 13:57:55	
CCV2	S	Reactive CN	P	254.5947	µg/l	8/26/2019 13:57:56	
CCB2	S	Reactive CN	P	-0.1729	µg/l	8/26/2019 13:57:57	
K4510-17	S	Reactive CN	P	-0.4321	µg/l	8/26/2019 13:57:58	
K4510-18	S	Reactive CN	P	-0.451	µg/l	8/26/2019 13:57:59	
K4510-19	S	Reactive CN	P	-0.7242	µg/l	8/26/2019 14:04:21	
K4510-20	S	Reactive CN	P	-0.5565	µg/l	8/26/2019 14:04:22	
K4510-21	S	Reactive CN	P	-0.2039	µg/l	8/26/2019 14:04:23	
PB122496BL	S	Reactive CN	P	-0.3963	µg/l	8/26/2019 14:04:24	
K4090-16DUP	S	Reactive CN	P	-0.4429	µg/l	8/26/2019 14:04:26	
K4487-01	S	Reactive CN	P	-0.4175	µg/l	8/26/2019 14:04:27	
K4090-16	S	Reactive CN	P	-0.0282	µg/l	8/26/2019 14:28:45	
CCV3	S	Reactive CN	P	265.5778	µg/l	8/26/2019 14:28:48	
CCB3	S	Reactive CN	P	-0.2935	µg/l	8/26/2019 14:28:50	