


LB104819

~~LB104796~~

RS 08-27-19

7471B

INSTRUMENT ID : CV1

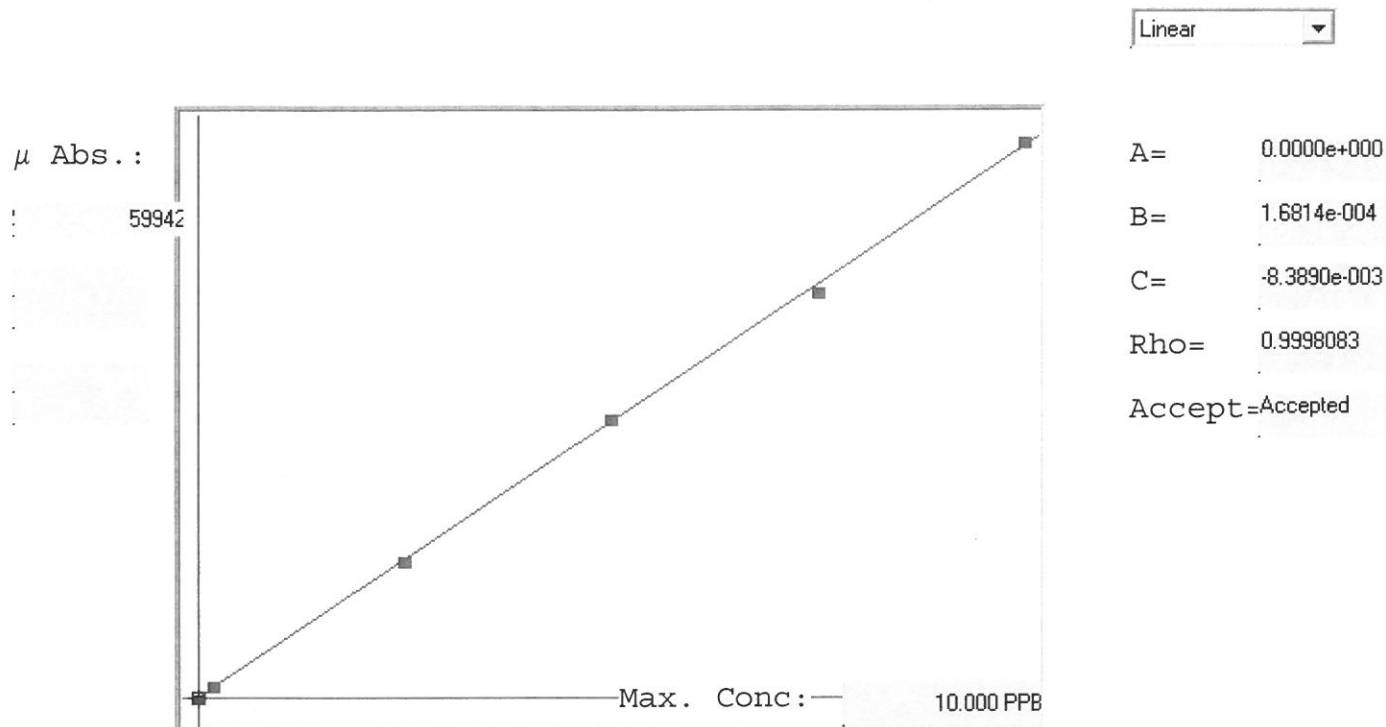

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.001	0.001	57	0.000	57				
0.2	0.200	0.208	0.008	1287	0.0 %	1287				
2.5	2.500	2.491	-0.009	14864	0.0 %	14864				
5.0	5.000	5.074	0.074	30228	0.0 %	30228				
7.5	7.500	7.356	-0.144	43799	0.0 %	43799				
10.0	10.000	10.070	0.070	59942	0.0 %	59942				

LB104819 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 26 Aug 2019 13:40:58				
Sample ID	Extended ID	µ Abs	Conc	Std Conc	Method	Units	Date	Type
0.0 - 1	50-0	57	-	0.0000	7471B	PPB	27 Aug 2019 13:40:49	S Std
0.2 - 1	50-2	1287	-	0.2000	7471B	PPB	27 Aug 2019 13:43:07	S Std
2.5 - 1	52-5	14864	-	2.5000	7471B	PPB	27 Aug 2019 13:45:26	S Std
5.0 - 1	55-0	30228	-	5.0000	7471B	PPB	27 Aug 2019 13:47:43	S Std
7.5 - 1	57-5	43799	-	7.5000	7471B	PPB	27 Aug 2019 13:50:00	S Std
10.0 - 1	510-0	59942	-	10.0000	7471B	PPB	27 Aug 2019 13:52:18	S Std
ICV87 - 1	ICV87	24017	4.0298	-	7471B	PPB	27 Aug 2019 13:56:42	U SMPL
ICB87 - 1	ICB87	7	-0.0072	-	7471B	PPB	27 Aug 2019 13:58:57	U SMPL
CCV01 - 1	CCV01	29794	5.0011	-	7471B	PPB	27 Aug 2019 14:01:13	U SMPL
CCB01 - 1	CCB01	-4	-0.0091	-	7471B	PPB	27 Aug 2019 14:03:29	U SMPL
CRA - 1	CRA	1256	0.2028	-	7471B	PPB	27 Aug 2019 14:05:45	U SMPL
HighStd - 1	HighStd	60182	10.1104	-	7471B	PPB	27 Aug 2019 14:08:01	U SMPL
ChkStd - 1	ChkStd	41184	6.9162	-	7471B	PPB	27 Aug 2019 14:10:16	U SMPL
PB122594BL - 1	PBS	-65	-0.0193	-	7471B	PPB	27 Aug 2019 14:12:35	U SMPL
PB122594BS - 1	LCSS	21182	3.5531	-	7471B	PPB	27 Aug 2019 14:14:52	U SMPL
K4086-05 - 1	NB-07-082619	649	0.1007	-	7471B	PPB	27 Aug 2019 14:17:08	U SMPL
K4088-08 - 1	CL-02-082619	7912	1.3219	-	7471B	PPB	27 Aug 2019 14:19:26	U SMPL
K4092-07 - 1	EO-02-082619	3413	0.5655	-	7471B	PPB	27 Aug 2019 14:21:44	U SMPL
K4093-03 - 1	PL-02-082619	1169	0.1882	-	7471B	PPB	27 Aug 2019 14:24:02	U SMPL
K4506-01 - 1	RO-COMP	7584	1.2668	-	7471B	PPB	27 Aug 2019 14:26:18	U SMPL
CCV02 - 1	CCV02	29793	5.0009	-	7471B	PPB	27 Aug 2019 14:28:34	U SMPL
CCB02 - 1	CCB02	-30	-0.0134	-	7471B	PPB	27 Aug 2019 14:30:51	U SMPL
K4514-02 - 1	S602-M-1.0-1.5-082319	1292	0.2088	-	7471B	PPB	27 Aug 2019 14:33:08	U SMPL
K4514-02DUP - 1	S602-M-1.0-1.5-082319DUP	1289	0.2083	-	7471B	PPB	27 Aug 2019 14:35:24	U SMPL
K4514-03 - 1	K4514-02MS	24064	4.0377	-	7471B	PPB	27 Aug 2019 14:37:39	U SMPL
K4514-04 - 1	K4514-02MSD	22853	3.8340	-	7471B	PPB	27 Aug 2019 14:39:55	U SMPL
K4516-07 - 1	T1-S-B1-B4	3247	0.5376	-	7471B	PPB	27 Aug 2019 14:42:13	U SMPL
K4516-10 - 1	T1-S-S-E	3548	0.5882	-	7471B	PPB	27 Aug 2019 14:44:30	U SMPL
K4516-17 - 1	T2-S-B1-B4	3361	0.5567	-	7471B	PPB	27 Aug 2019 14:46:47	U SMPL
K4516-20 - 1	T2-S-D	13821	2.3154	-	7471B	PPB	27 Aug 2019 14:49:05	U SMPL
K4524-03 - 1	TT-013-IDWSO-20190823	109	0.0099	-	7471B	PPB	27 Aug 2019 14:51:23	U SMPL
K4525-01 - 1	T9-12-13-A1-A4(0-1.9)	61891	10.3978	-	7471B	PPB	27 Aug 2019 14:53:39	U SMPL
CCV03 - 1	CCV03	29982	5.0327	-	7471B	PPB	27 Aug 2019 14:55:55	U SMPL
CCB03 - 1	CCB03	-45	-0.0160	-	7471B	PPB	27 Aug 2019 14:58:12	U SMPL
K4525-10 - 1	T9-12-13-B1-B4(0-1.9)	90123	15.1446	-	7471B	PPB	27 Aug 2019 15:00:30	U SMPL
K4525-19 - 1	T9-12-13-C(0-1.9)	1130	0.1816	-	7471B	PPB	27 Aug 2019 15:02:46	U SMPL
K4526-02 - 1	T9-12-13-D(0-1.9)	1648	0.2687	-	7471B	PPB	27 Aug 2019 15:05:05	U SMPL
K4526-05 - 1	T9-12-13-F1-F4(0-1.9)	6626	1.1057	-	7471B	PPB	27 Aug 2019 15:07:21	U SMPL
K4526-14 - 1	T9-12-13-G1-G4(0-1.9)	937	0.1492	-	7471B	PPB	27 Aug 2019 15:09:37	U SMPL
K4526-19 - 1	T9-12-13-L(0-1.9)	7198	1.2019	-	7471B	PPB	27 Aug 2019 15:11:54	U SMPL
PB122595BL - 1	PBS	4	-0.0077	-	7471B	PPB	27 Aug 2019 15:14:11	U SMPL
PB122595BS - 1	LCSS	21320	3.5763	-	7471B	PPB	27 Aug 2019 15:16:29	U SMPL
K4527-02 - 1	T9-12-13-M(0-1.9)	15531	2.6029	-	7471B	PPB	27 Aug 2019 15:18:47	U SMPL
K4527-02DUP - 1	T9-12-13-M(0-1.9)DUP	15367	2.5754	-	7471B	PPB	27 Aug 2019 15:21:02	U SMPL
CCV04 - 1	CCV04	30924	5.1911	-	7471B	PPB	27 Aug 2019 15:23:19	U SMPL
CCB04 - 1	CCB04	-20	-0.0118	-	7471B	PPB	27 Aug 2019 15:25:35	U SMPL
K4527-02MS - 1	T9-12-13-M(0-1.9)MS	39766	6.6778	-	7471B	PPB	27 Aug 2019 15:27:52	U SMPL
K4527-02MSD - 1	T9-12-13-M(0-1.9)MSD	38103	6.3981	-	7471B	PPB	27 Aug 2019 15:30:09	U SMPL
K4527-05 - 1	T9-12-13-N1-N4(0-1.9)	41438	6.9589	-	7471B	PPB	27 Aug 2019 15:32:26	U SMPL
K4527-14 - 1	T9-12-13-O(0-1.9)	46281	7.7732	-	7471B	PPB	27 Aug 2019 15:34:42	U SMPL
K4527-17 - 1	T9-12-13-P(0-1.9)	400	0.0589	-	7471B	PPB	27 Aug 2019 15:37:00	U SMPL
K4527-20 - 1	T9-12-13-Q2-Q4(0-1.9)	4463	0.7420	-	7471B	PPB	27 Aug 2019 15:39:19	U SMPL
K4528-07 - 1	T9-12-13-R(0-1.9)	4113	0.6832	-	7471B	PPB	27 Aug 2019 15:41:37	U SMPL
K4528-10 - 1	T9-12-13-S1-S4(0-1.9)	8621	1.4411	-	7471B	PPB	27 Aug 2019 15:43:56	U SMPL
K4528-19 - 1	T9-12-13-T1-T4(0-1.9)	1925	0.3153	-	7471B	PPB	27 Aug 2019 15:46:20	U SMPL
K4536-01 - 1	SB-1-15-17	624	0.0965	-	7471B	PPB	27 Aug 2019 15:48:37	U SMPL
CCV05 - 1	CCV05	31087	5.2185	-	7471B	PPB	27 Aug 2019 15:50:54	U SMPL
CCB05 - 1	CCB05	-24	-0.0124	-	7471B	PPB	27 Aug 2019 15:53:11	U SMPL
K4536-03 - 1	SB-1-20-22	403	0.0594	-	7471B	PPB	27 Aug 2019 15:55:27	U SMPL
K4536-05 - 1	SB-1-25-27	1144	0.1840	-	7471B	PPB	27 Aug 2019 15:57:43	U SMPL
K4536-07 - 1	SB-1-30-32	1463	0.2376	-	7471B	PPB	27 Aug 2019 16:00:00	U SMPL
K4543-03 - 1	TP-2-S	4833	0.8042	-	7471B	PPB	27 Aug 2019 16:02:16	U SMPL
K4543-07 - 1	TP-2-D	3199	0.5295	-	7471B	PPB	27 Aug 2019 16:04:33	U SMPL
K4543-11 - 1	TP-3-S	1242	0.2004	-	7471B	PPB	27 Aug 2019 16:06:50	U SMPL
K4543-15 - 1	TP-9-S	871	0.1381	-	7471B	PPB	27 Aug 2019 16:09:10	U SMPL
K4514-02LX5 - 1		283	0.0392	-	7471B	PPB	27 Aug 2019 16:11:32	U SMPL
K4514-02A - 1		23596	3.9590	-	7471B	PPB	27 Aug 2019 16:13:50	U SMPL
K4527-02LX5 - 1		2850	0.4708	-	7471B	PPB	27 Aug 2019 16:16:07	U SMPL
CCV06 - 1	CCV06	30889	5.1852	-	7471B	PPB	27 Aug 2019 16:18:24	U SMPL
CCB06 - 1	CCB06	-35	-0.0143	-	7471B	PPB	27 Aug 2019 16:20:41	U SMPL
K4527-02A - 1		39393	6.6150	-	7471B	PPB	27 Aug 2019 16:22:57	U SMPL
K4525-01DLX2 - 1		30198	5.0690	-	7471B	PPB	27 Aug 2019 16:25:15	U SMPL
K4525-10DLX3 - 1		29882	5.0159	-	7471B	PPB	27 Aug 2019 16:27:32	U SMPL
CCV07 - 1	CCV07	29370	4.9298	-	7471B	PPB	27 Aug 2019 16:29:50	U SMPL
CCB07 - 1	CCB07	-18	-0.0114	-	7471B	PPB	27 Aug 2019 16:32:06	U SMPL