


LB104862

7470A

INSTRUMENT ID: CV1

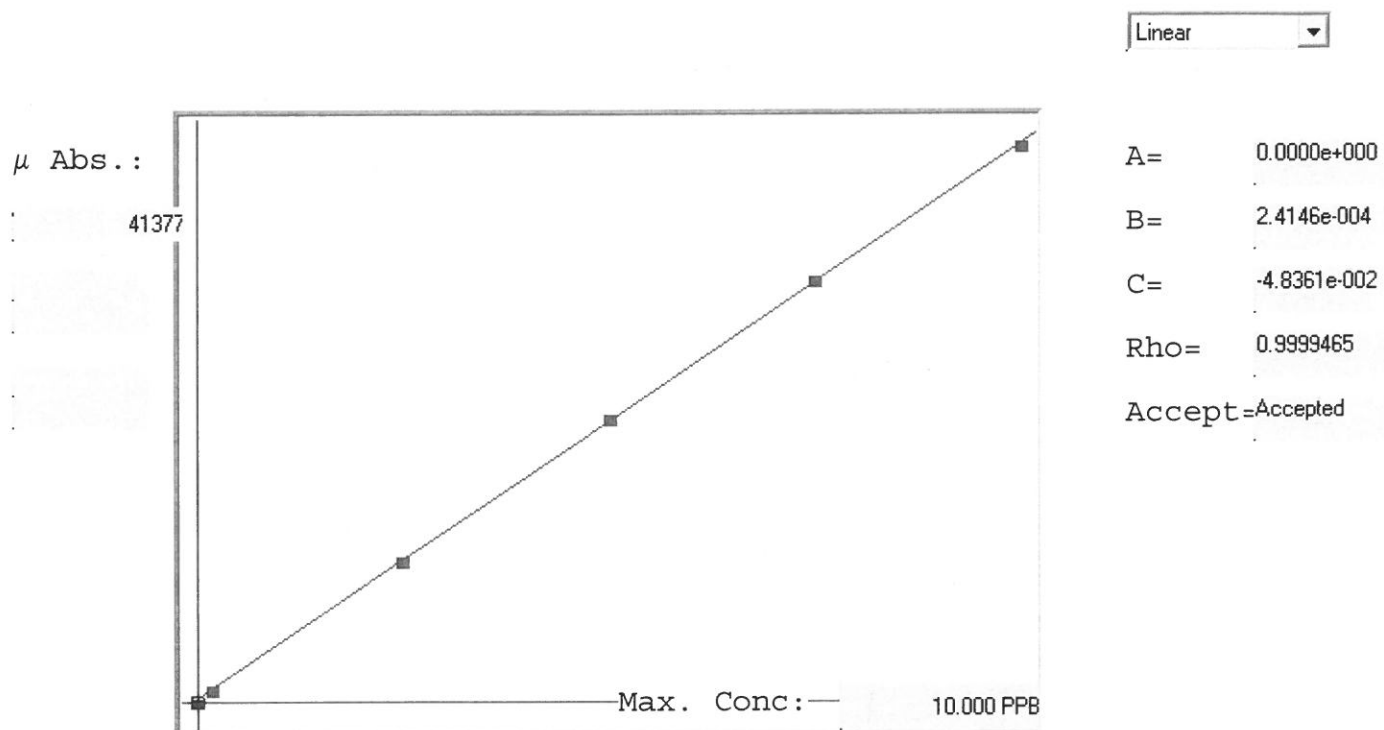

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.022	-0.022	108	0.000	108				
0.2	0.200	0.183	-0.017	958	0.0 %	958				
2.5	2.500	2.503	0.003	10565	0.0 %	10565				
5.0	5.000	5.057	0.057	21145	0.0 %	21145				
7.5	7.500	7.537	0.037	31414	0.0 %	31414				
10.0	10.000	9.943	-0.057	41377	0.0 %	41377				

LB104862 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 29 Aug 2019 10:01:13							
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type		
0.0 - 1	500	108	-	0.00007470A	PPB		29 Aug 2019 10:05:55	S	Std		
0.2 - 1	50-2	958	-	0.20007470A	PPB		29 Aug 2019 10:08:03	S	Std		
2.5 - 1	52-5	10565	-	2.50007470A	PPB		29 Aug 2019 10:10:12	S	Std		
5.0 - 1	55-0	21145	-	5.00007470A	PPB		29 Aug 2019 10:12:21	S	Std		
7.5 - 1	57-5	31414	-	7.50007470A	PPB		29 Aug 2019 10:14:29	S	Std		
10.0 - 1	510-0	41377	-	10.00007470A	PPB		29 Aug 2019 10:16:36	S	Std		
ICV91 - 1	ICV91	16444	3.9222	-7470A	PPB		29 Aug 2019 10:21:45	U	SMPL		
ICB91 - 1	ICB91	75	-0.0303	-7470A	PPB		29 Aug 2019 10:23:51	U	SMPL		
CCV21 - 1	CCV21	20369	4.8699	-7470A	PPB		29 Aug 2019 10:25:57	U	SMPL		
CCB21 - 1	CCB21	66	-0.0324	-7470A	PPB		29 Aug 2019 10:28:03	U	SMPL		
CRA - 1	CRA	928	0.1757	-7470A	PPB		29 Aug 2019 10:30:11	U	SMPL		
HighStd - 1	HighStd	40879	9.8223	-7470A	PPB		29 Aug 2019 10:32:17	U	SMPL		
ChkStd - 1	ChkStd	28525	6.8393	-7470A	PPB		29 Aug 2019 10:34:24	U	SMPL		
PB122656BL - 1	PBW	78	-0.0295	-7470A	PPB		29 Aug 2019 10:36:31	U	SMPL		
PB122656BS - 1	LCSW	16324	3.8932	-7470A	PPB		29 Aug 2019 10:38:39	U	SMPL		
K4517-23 - 1	T2-S-A1-A4	115	-0.0206	-7470A	PPB		29 Aug 2019 10:40:47	U	SMPL		
K4517-30 - 1	T4-S-D1-D4	131	-0.0167	-7470A	PPB		29 Aug 2019 10:42:55	U	SMPL		
K4517-33 - 1	T4-S-C	134	-0.0160	-7470A	PPB		29 Aug 2019 10:45:03	U	SMPL		
K4517-36 - 1	T4-S-E	128	-0.0175	-7470A	PPB		29 Aug 2019 10:47:12	U	SMPL		
K4526-22 - 1	T9-12-13-D(0-1.9)	134	-0.0160	-7470A	PPB		29 Aug 2019 10:49:19	U	SMPL		
CCV22 - 1	CCV22	20172	4.8224	-7470A	PPB		29 Aug 2019 10:51:25	U	SMPL		
CCB22 - 1	CCB22	81	-0.0288	-7470A	PPB		29 Aug 2019 10:53:32	U	SMPL		
K4526-22DUP - 1	T9-12-13-D(0-1.9)DUP	140	-0.0146	-7470A	PPB		29 Aug 2019 10:55:39	U	SMPL		
K4526-22MS - 1	T9-12-13-D(0-1.9)MS	16521	3.9408	-7470A	PPB		29 Aug 2019 10:57:46	U	SMPL		
K4526-22MSD - 1	T9-12-13-D(0-1.9)MSD	16710	3.9864	-7470A	PPB		29 Aug 2019 10:59:52	U	SMPL		
K4526-25 - 1	T9-12-13-F1-F4(0-1.9)	105	-0.0230	-7470A	PPB		29 Aug 2019 11:02:00	U	SMPL		
K4526-34 - 1	T9-12-13-G1-G4(0-1.9)	124	-0.0184	-7470A	PPB		29 Aug 2019 11:04:07	U	SMPL		
K4526-39 - 1	T9-12-13-L(0-1.9)	132	-0.0165	-7470A	PPB		29 Aug 2019 11:06:15	U	SMPL		
K4527-22 - 1	T9-12-13-M(0-1.9)	128	-0.0175	-7470A	PPB		29 Aug 2019 11:08:23	U	SMPL		
K4527-25 - 1	T9-12-13-N1-N4(0-1.9)	137	-0.0153	-7470A	PPB		29 Aug 2019 11:10:32	U	SMPL		
K4527-34 - 1	T9-12-13-O(0-1.9)	143	-0.0138	-7470A	PPB		29 Aug 2019 11:12:40	U	SMPL		
K4527-37 - 1	T9-12-13-P(0-1.9)	147	-0.0129	-7470A	PPB		29 Aug 2019 11:14:48	U	SMPL		
CCV23 - 1	CCV23	20376	4.8716	-7470A	PPB		29 Aug 2019 11:16:55	U	SMPL		
CCB23 - 1	CCB23	77	-0.0298	-7470A	PPB		29 Aug 2019 11:19:01	U	SMPL		
K4527-40 - 1	T9-12-13-Q2-Q4(0-1.9)	104	-0.0232	-7470A	PPB		29 Aug 2019 11:21:08	U	SMPL		
K4544-21 - 1	T16-17-B1-B4-(0-2.25)	117	-0.0201	-7470A	PPB		29 Aug 2019 11:23:15	U	SMPL		
K4544-30 - 1	T16-17-C1-C4-(0-2.25)	137	-0.0153	-7470A	PPB		29 Aug 2019 11:25:22	U	SMPL		
K4544-39 - 1	T16-17-E1-E4-(0-2.25)7-	159	-0.0100	-7470A	PPB		29 Aug 2019 11:27:29	U	SMPL		
K4546-29 - 1	T3-S-C1-C4	161	-0.0095	-7470A	PPB		29 Aug 2019 11:29:36	U	SMPL		
K4546-32 - 1	T3-S-A	146	-0.0131	-7470A	PPB		29 Aug 2019 11:31:44	U	SMPL		
K4548-18 - 1	T8-S-G1-G4(0)	141	-0.0143	-7470A	PPB		29 Aug 2019 11:33:52	U	SMPL		
K4559-01 - 1	SOIL-SAMPLE-4	138	-0.0150	-7470A	PPB		29 Aug 2019 11:36:00	U	SMPL		
PB122657BL - 1	PBW	144	-0.0136	-7470A	PPB		29 Aug 2019 11:38:08	U	SMPL		
PB122657BS - 1	LCSW	16577	3.9543	-7470A	PPB		29 Aug 2019 11:40:16	U	SMPL		
CCV24 - 1	CCV24	19968	4.7731	-7470A	PPB		29 Aug 2019 11:42:23	U	SMPL		
CCB24 - 1	CCB24	89	-0.0269	-7470A	PPB		29 Aug 2019 11:44:31	U	SMPL		
K4567-06 - 1	TP-7-S	135	-0.0158	-7470A	PPB		29 Aug 2019 11:46:37	U	SMPL		
K4567-06DUP - 1	TP-7-SDUP	131	-0.0167	-7470A	PPB		29 Aug 2019 11:48:44	U	SMPL		
K4567-06MS - 1	TP-7-SMS	16521	3.9408	-7470A	PPB		29 Aug 2019 11:50:51	U	SMPL		
K4567-06MSD - 1	TP-7-SMSD	17645	4.2122	-7470A	PPB		29 Aug 2019 11:52:58	U	SMPL		
K4567-12 - 1	TP-7-D	117	-0.0201	-7470A	PPB		29 Aug 2019 11:55:05	U	SMPL		
K4567-16 - 1	TP-8-S	180	-0.0049	-7470A	PPB		29 Aug 2019 11:57:12	U	SMPL		
K4567-20 - 1	TP-8-D	149	-0.0124	-7470A	PPB		29 Aug 2019 11:59:21	U	SMPL		
K4571-03 - 1	RT-3424	166	-0.0083	-7470A	PPB		29 Aug 2019 12:01:29	U	SMPL		
K4571-06 - 1	RBR-200028	152	-0.0117	-7470A	PPB		29 Aug 2019 12:03:37	U	SMPL		
K4571-09 - 1	RBR-200052	165	-0.0085	-7470A	PPB		29 Aug 2019 12:05:44	U	SMPL		
CCV25 - 1	CCV25	20260	4.8436	-7470A	PPB		29 Aug 2019 12:07:51	U	SMPL		
CCB25 - 1	CCB25	88	-0.0271	-7470A	PPB		29 Aug 2019 12:09:58	U	SMPL		
PB122658BL - 1	PBW	145	-0.0133	-7470A	PPB		29 Aug 2019 12:12:06	U	SMPL		
PB122658BS - 1	LCSW	16542	3.9459	-7470A	PPB		29 Aug 2019 12:14:13	U	SMPL		
K4543-18 - 1	TP-2-GW	146	-0.0131	-7470A	PPB		29 Aug 2019 12:16:20	U	SMPL		
K4543-18DUP - 1	TP-2-GWDUP	165	-0.0085	-7470A	PPB		29 Aug 2019 12:18:27	U	SMPL		
K4543-18MS - 1	TP-2-GWMS	16297	3.8867	-7470A	PPB		29 Aug 2019 12:20:35	U	SMPL		
K4543-18MSD - 1	TP-2-GWMSD	16359	3.9017	-7470A	PPB		29 Aug 2019 12:22:42	U	SMPL		
K4567-22 - 1	TP-7-GW	135	-0.0158	-7470A	PPB		29 Aug 2019 12:24:50	U	SMPL		
K4567-25 - 1	TP-8-GW	170	-0.0073	-7470A	PPB		29 Aug 2019 12:26:58	U	SMPL		
PB122656TB - 1	PB122604TB	150	-0.0121	-7470A	PPB		29 Aug 2019 12:29:07	U	SMPL		
PB122657TB - 1	PB122606TB	141	-0.0143	-7470A	PPB		29 Aug 2019 12:31:14	U	SMPL		
CCV26 - 1	CCV26	20111	4.8076	-7470A	PPB		29 Aug 2019 12:33:22	U	SMPL		
CCB26 - 1	CCB26	96	-0.0252	-7470A	PPB		29 Aug 2019 12:35:29	U	SMPL		
PB122658TB - 1	PB122607TB	84	-0.0281	-7470A	PPB		29 Aug 2019 12:37:36	U	SMPL		
K4526-22LX5 - 1		109	-0.0220	-7470A	PPB		29 Aug 2019 12:53:41	U	SMPL		
K4526-22A - 1		16948	4.0439	-7470A	PPB		29 Aug 2019 12:55:47	U	SMPL		
K4567-06LX5 - 1		69	-0.0317	-7470A	PPB		29 Aug 2019 12:57:55	U	SMPL		
K4567-06A - 1		17827	4.2561	-7470A	PPB		29 Aug 2019 13:00:02	U	SMPL		
K4543-18LX5 - 1		92	-0.0261	-7470A	PPB		29 Aug 2019 13:02:09	U	SMPL		
K4543-18A - 1		16969	4.0490	-7470A	PPB		29 Aug 2019 13:04:17	U	SMPL		
CCV27 - 1	CCV27	20741	4.9598	-7470A	PPB		29 Aug 2019 13:06:25	U	SMPL		
CCB27 - 1	CCB27	110	-0.0218	-7470A	PPB		29 Aug 2019 13:08:34	U	SMPL		