


LB104892

245.1

INSTRUMENT ID : CV1

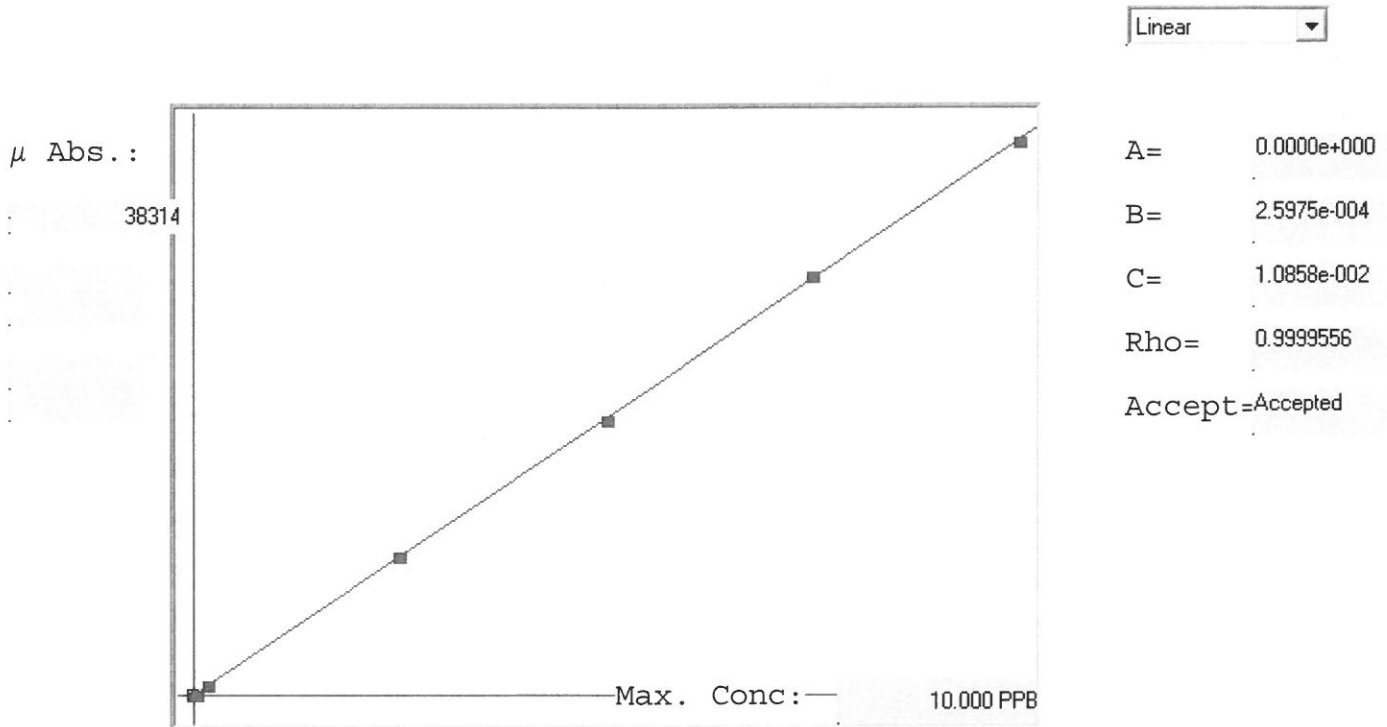

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.014	-0.014	-96	0.000	-96				
0.05	0.050	0.038	-0.012	103	0.0 %	103				
0.2	0.200	0.214	0.014	781	0.0 %	781				
2.5	2.500	2.523	0.023	9671	0.0 %	9671				
5.0	5.000	4.960	-0.040	19052	0.0 %	19052				
7.5	7.500	7.567	0.067	29090	0.0 %	29090				
10.0	10.000	9.963	-0.037	38314	0.0 %	38314				

LB104892 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 30 Aug 2019 11:55:00

Sample ID	Extended ID	μ Abs.	Conc.	Std Cond	Method	Units	Date	Type	Type
0.0 - 1	50-0	-96	-	0.0000	245.1	PPB	30 Aug 2019 12:20:46	S	Std
0.05 - 1	50-05	103	-	0.0500	245.1	PPB	30 Aug 2019 12:23:04	S	Std
0.2 - 1	50-2	781	-	0.2000	245.1	PPB	30 Aug 2019 12:25:22	S	Std
2.5 - 1	52-5	9671	-	2.5000	245.1	PPB	30 Aug 2019 12:27:40	S	Std
5.0 - 1	55-0	19052	-	5.0000	245.1	PPB	30 Aug 2019 12:29:58	S	Std
7.5 - 1	57-5	29090	-	7.5000	245.1	PPB	30 Aug 2019 12:32:15	S	Std
10.0 - 1	516-0	38314	-	10.0000	245.1	PPB	30 Aug 2019 12:41:08	S	Std
ICV95 - 1	ICV95	14714	3.8329	-245.1		PPB	30 Aug 2019 12:43:59	U	SMPL
ICB95 - 1	ICB95	-48	-0.0016	-245.1		PPB	30 Aug 2019 12:46:14	U	SMPL
CCV36 - 1	CCV36	18796	4.8932	-245.1		PPB	30 Aug 2019 12:48:31	U	SMPL
CCB36 - 1	CCB36	-68	-0.0068	-245.1		PPB	30 Aug 2019 12:50:46	U	SMPL
CRA - 1	CRA	78	0.0311	-245.1		PPB	30 Aug 2019 12:53:02	U	SMPL
HighStd - 1	HighStd	37362	9.7158	-245.1		PPB	30 Aug 2019 12:55:18	U	SMPL
ChkStd - 1	ChkStd	26398	6.8678	-245.1		PPB	30 Aug 2019 12:57:34	U	SMPL
PB122711BL - 1	PBW	-42	-0.0001	-245.1		PPB	30 Aug 2019 12:59:53	U	SMPL
PB122711BS - 1	LCSW	16617	4.3272	-245.1		PPB	30 Aug 2019 13:02:10	U	SMPL
K4555-23 - 1	TW-10-DEP	3050	0.8031	-245.1		PPB	30 Aug 2019 13:04:27	U	SMPL
K4577-01 - 1	GW-1	55	0.0251	-245.1		PPB	30 Aug 2019 13:06:45	U	SMPL
K4577-01DUP - 1	GW-1DUP	87	0.0335	-245.1		PPB	30 Aug 2019 13:09:03	U	SMPL
K4577-01MS - 1	GW-1MS	17663	4.5989	-245.1		PPB	30 Aug 2019 13:11:21	U	SMPL
K4577-01MSD - 1	GW-1MSD	17497	4.5558	-245.1		PPB	30 Aug 2019 13:13:37	U	SMPL
CCV37 - 1	CCV37	19037	4.9558	-245.1		PPB	30 Aug 2019 13:15:53	U	SMPL
CCB37 - 1	CCB37	-24	0.0046	-245.1		PPB	30 Aug 2019 13:18:09	U	SMPL
K4615-01 - 1	NR-KIT-TAP-NEW-FILTER	22	0.0166	-245.1		PPB	30 Aug 2019 13:20:25	U	SMPL
K4577-01LX5 - 1		23	0.0168	-245.1		PPB	30 Aug 2019 13:22:41	U	SMPL
K4577-01A - 1		17351	4.5178	-245.1		PPB	30 Aug 2019 13:24:58	U	SMPL
CCV38 - 1	CCV38	18362	4.7804	-245.1		PPB	30 Aug 2019 13:27:14	U	SMPL
CCB38 - 1	CCB38	-28	0.0036	-245.1		PPB	30 Aug 2019 13:29:31	U	SMPL