


LBID4948

7471B

INSTRUMENT ID : CU1

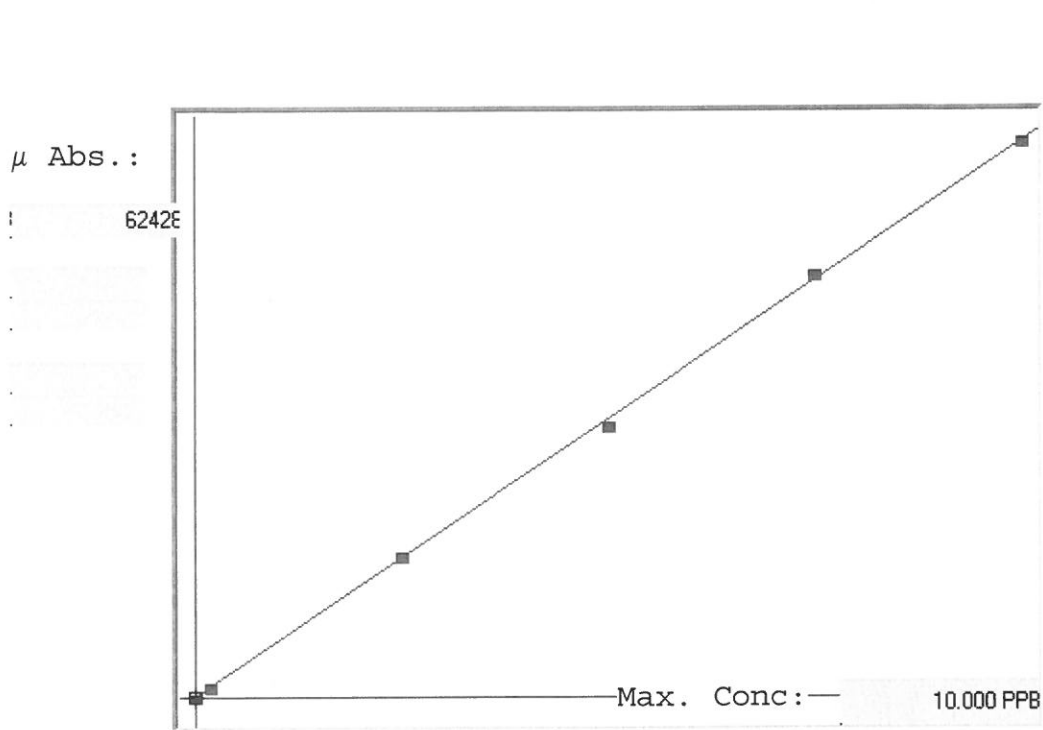

Linear

A= 0.0000e+000

B= 1.5992e-004

C= -4.5057e-003

Rho= 0.9998165

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.017	0.017	132	0.000	132				
0.2	0.200	0.191	-0.009	1224	0.0 %	1224				
2.5	2.500	2.549	0.049	15970	0.0 %	15970				
5.0	5.000	4.868	-0.132	30468	0.0 %	30468				
7.5	7.500	7.596	0.096	47530	0.0 %	47530				
10.0	10.000	9.979	-0.021	62428	0.0 %	62428				

LB104948 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 04 Sep 2019 13:44:26					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SD-0	132	-	0.0000	7471B	PPB	04 Sep 2019 13:51:46	S	Std
0.2 - 1	SD-2	1224	-	0.2000	7471B	PPB	04 Sep 2019 13:54:05	S	Std
2.5 - 1	SD-5	15970	-	2.5000	7471B	PPB	04 Sep 2019 13:56:23	S	Std
5.0 - 1	SD-0	30468	-	5.0000	7471B	PPB	04 Sep 2019 13:58:41	S	Std
7.5 - 1	SD-5	47530	-	7.5000	7471B	PPB	04 Sep 2019 14:00:59	S	Std
10.0 - 1	SD-0	62428	-	10.0000	7471B	PPB	04 Sep 2019 14:03:16	S	Std
ICV02 - 1	ICV02	24950	3.9854	-	7471B	PPB	04 Sep 2019 14:08:22	U	SMPL
ICB02 - 1	ICB02	91	0.0100	-	7471B	PPB	04 Sep 2019 14:10:37	U	SMPL
CCV71 - 1	CCV71	30391	4.8555	-	7471B	PPB	04 Sep 2019 14:12:53	U	SMPL
CCB71 - 1	CCB71	49	0.0033	-	7471B	PPB	04 Sep 2019 14:15:10	U	SMPL
CRA - 1	CRA	1213	0.1895	-	7471B	PPB	04 Sep 2019 14:17:26	U	SMPL
HighStd - 1	HighStd	62272	9.9538	-	7471B	PPB	04 Sep 2019 14:19:42	U	SMPL
ChkStd - 1	ChkStd	43999	7.0316	-	7471B	PPB	04 Sep 2019 14:21:59	U	SMPL
PB122806BL - 1	PB122806BL	7	-0.0034	-	7471B	PPB	04 Sep 2019 14:24:16	U	SMPL
PB122806BS - 1	LCSS	21644	3.4567	-	7471B	PPB	04 Sep 2019 14:26:34	U	SMPL
K4639-03 - 1	DW-01	1549	0.2432	-	7471B	PPB	04 Sep 2019 14:28:51	U	SMPL
K4639-04 - 1	DW-02	7423	1.1825	-	7471B	PPB	04 Sep 2019 14:31:09	U	SMPL
K4639-05 - 1	DW-03	430	0.0643	-	7471B	PPB	04 Sep 2019 14:33:26	U	SMPL
K4639-06 - 1	SS-01	818	0.1263	-	7471B	PPB	04 Sep 2019 14:35:44	U	SMPL
K4643-01 - 1	T11-B1-B4-(0-4)	4713	0.7492	-	7471B	PPB	04 Sep 2019 14:38:00	U	SMPL
CCV72 - 1	CCV72	30619	4.8920	-	7471B	PPB	04 Sep 2019 14:40:15	U	SMPL
CCB72 - 1	CCB72	59	0.0049	-	7471B	PPB	04 Sep 2019 14:42:31	U	SMPL
K4643-01DUP - 1	T11-B1-B4-(0-4)DUP	4731	0.7521	-	7471B	PPB	04 Sep 2019 14:44:48	U	SMPL
K4643-01MS - 1	T11-B1-B4-(0-4)MS	25478	4.0698	-	7471B	PPB	04 Sep 2019 14:47:04	U	SMPL
K4643-01MSD - 1	T11-B1-B4-(0-4)MSD	26064	4.1635	-	7471B	PPB	04 Sep 2019 14:49:20	U	SMPL
K4643-10 - 1	T11-C1-C4-(0-4)	2914	0.4615	-	7471B	PPB	04 Sep 2019 14:51:36	U	SMPL
K4643-19 - 1	T11-D1-D4-(0-4)	6916	1.1015	-	7471B	PPB	04 Sep 2019 14:53:53	U	SMPL
K4644-08 - 1	T11-E1-E4-(0-4)	13513	2.1564	-	7471B	PPB	04 Sep 2019 14:56:10	U	SMPL
K4655-03 - 1	TP-15-S	2129	0.3360	-	7471B	PPB	04 Sep 2019 14:58:28	U	SMPL
K4655-07 - 1	TP-15-D	1752	0.2757	-	7471B	PPB	04 Sep 2019 15:00:45	U	SMPL
K4668-01 - 1	SU-04-090319	3764	0.5974	-	7471B	PPB	04 Sep 2019 15:03:04	U	SMPL
K4643-01LX5 - 1		1009	0.1568	-	7471B	PPB	04 Sep 2019 15:05:20	U	SMPL
CCV73 - 1	CCV73	30855	4.9297	-	7471B	PPB	04 Sep 2019 15:07:36	U	SMPL
CCB73 - 1	CCB73	56	0.0044	-	7471B	PPB	04 Sep 2019 15:09:53	U	SMPL
K4643-01A - 1		25478	4.0698	-	7471B	PPB	04 Sep 2019 15:12:10	U	SMPL
CCV74 - 1	CCV74	32112	5.1307	-	7471B	PPB	04 Sep 2019 15:14:27	U	SMPL
CCB74 - 1	CCB74	78	0.0080	-	7471B	PPB	04 Sep 2019 15:16:46	U	SMPL