


LB104985

7471B

INSTRUMENT ID : CV1

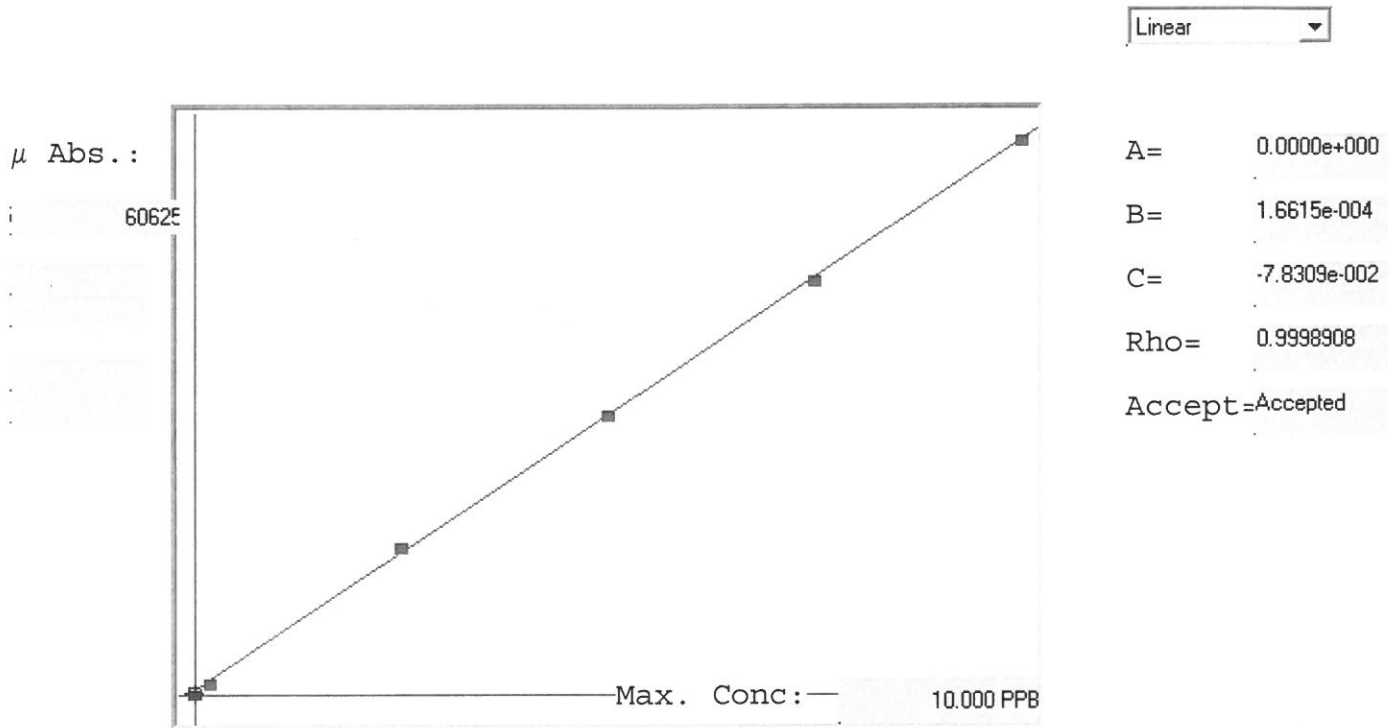

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.041	-0.041	224	0.000	224				
0.2	0.200	0.161	-0.039	1440	0.0 %	1440				
2.5	2.500	2.614	0.114	16202	0.0 %	16202				
5.0	5.000	5.012	0.012	30635	0.0 %	30635				
7.5	7.500	7.461	-0.039	45375	0.0 %	45375				
10.0	10.000	9.994	-0.006	60625	0.0 %	60625				

LB104985 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 06 Sep 2019 09:38:25

Sample ID	Extended ID	μ Abs	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SC-0	224	-	0.0007471B	-	PPB	06 Sep 2019 09:48:55	S	Std
0.2 - 1	SC-2	1440	-	0.20007471B	-	PPB	06 Sep 2019 09:51:13	S	Std
2.5 - 1	SC-5	16202	-	2.50007471B	-	PPB	06 Sep 2019 09:53:31	S	Std
5.0 - 1	SC-0	30635	-	5.00007471B	-	PPB	06 Sep 2019 09:55:49	S	Std
7.5 - 1	SC-5	45375	-	7.50007471B	-	PPB	06 Sep 2019 09:58:06	S	Std
10.0 - 1	SC-0	60625	-	10.00007471B	-	PPB	06 Sep 2019 10:00:22	S	Std
ICV04 - 1	ICV04	24942	4.0657	-7471B	-	PPB	06 Sep 2019 10:06:32	U	SMPL
ICB04 - 1	ICB04	149	-0.0536	-7471B	-	PPB	06 Sep 2019 10:08:52	U	SMPL
CCV78 - 1	CCV78	30300	4.9559	-7471B	-	PPB	06 Sep 2019 10:11:08	U	SMPL
CCB78 - 1	CCB78	140	-0.0550	-7471B	-	PPB	06 Sep 2019 10:13:24	U	SMPL
CRA - 1	CRA	1403	0.1548	-7471B	-	PPB	06 Sep 2019 10:15:40	U	SMPL
HighStd - 1	HighStd	60640	9.9968	-7471B	-	PPB	06 Sep 2019 10:17:56	U	SMPL
ChkStd - 1	ChkStd	41347	6.7914	-7471B	-	PPB	06 Sep 2019 10:20:13	U	SMPL
PB122857BL - 1	PBS	174	-0.0494	-7471B	-	PPB	06 Sep 2019 10:22:41	U	SMPL
PB122857BS - 1	LCSS	23128	3.7643	-7471B	-	PPB	06 Sep 2019 10:25:04	U	SMPL
K4522-01 - 1	SIDEWALL-4	5733	0.8742	-7471B	-	PPB	06 Sep 2019 10:27:22	U	SMPL
K4522-05 - 1	BOTTOM-5	1795	0.2199	-7471B	-	PPB	06 Sep 2019 10:29:39	U	SMPL
K4650-01 - 1	TP-1	7133	1.1068	-7471B	-	PPB	06 Sep 2019 10:31:56	U	SMPL
K4650-03 - 1	TP-2	31917	5.2246	-7471B	-	PPB	06 Sep 2019 10:34:14	U	SMPL
K4650-05 - 1	TP-3	12698	2.0314	-7471B	-	PPB	06 Sep 2019 10:36:30	U	SMPL
CCV79 - 1	CCV79	30154	4.9317	-7471B	-	PPB	06 Sep 2019 10:38:46	U	SMPL
CCB79 - 1	CCB79	130	-0.0567	-7471B	-	PPB	06 Sep 2019 10:41:02	U	SMPL
K4650-07 - 1	TP-4	26736	4.3638	-7471B	-	PPB	06 Sep 2019 10:43:18	U	SMPL
K4650-09 - 1	TP-5	1109	0.1059	-7471B	-	PPB	06 Sep 2019 10:45:34	U	SMPL
K4650-11 - 1	TP-6	624	0.0254	-7471B	-	PPB	06 Sep 2019 10:47:50	U	SMPL
K4650-13 - 1	TP-7	9275	1.4627	-7471B	-	PPB	06 Sep 2019 10:50:07	U	SMPL
K4650-15 - 1	TP-8	85711	14.1623	-7471B	-	PPB	06 Sep 2019 10:52:23	U	SMPL
K4680-01 - 1	T1-1-4-(0-1.5)	7368	1.1459	-7471B	-	PPB	06 Sep 2019 10:54:40	U	SMPL
K4680-08 - 1	T2-3-(2-4)	1575	0.1834	-7471B	-	PPB	06 Sep 2019 10:56:59	U	SMPL
K4680-11 - 1	T3-1-4-(0-1.5)	35528	5.8246	-7471B	-	PPB	06 Sep 2019 10:59:16	U	SMPL
K4683-01 - 1	20190663-LOCATION-1	158199	26.2060	-7471B	-	PPB	06 Sep 2019 11:01:34	U	SMPL
K4683-01DUP - 1	20190663-LOCATION-1DUP	159526	26.4264	-7471B	-	PPB	06 Sep 2019 11:03:50	U	SMPL
CCV80 - 1	CCV80	30212	4.9413	-7471B	-	PPB	06 Sep 2019 11:06:08	U	SMPL
CCB80 - 1	CCB80	121	-0.0582	-7471B	-	PPB	06 Sep 2019 11:08:27	U	SMPL
K4683-01MS - 1	20190663-LOCATION-1MS	175686	29.1114	-7471B	-	PPB	06 Sep 2019 11:15:10	U	SMPL
K4683-01MSD - 1	20190663-LOCATION-1MSD	173025	28.6692	-7471B	-	PPB	06 Sep 2019 11:17:26	U	SMPL
K4683-02 - 1	20190664-LOCATION-2	48881	8.0431	-7471B	-	PPB	06 Sep 2019 11:19:44	U	SMPL
K4683-03 - 1	20190665-LOCATION-3	74554	12.3086	-7471B	-	PPB	06 Sep 2019 11:22:03	U	SMPL
K4683-04 - 1	20190666-FIELD-DUPLICATE	86018	14.2133	-7471B	-	PPB	06 Sep 2019 11:24:21	U	SMPL
K4694-01 - 1	T1-1-4-(0-1.5)	14546	2.3385	-7471B	-	PPB	06 Sep 2019 11:26:39	U	SMPL
K4694-10 - 1	T2-1-4-(0-1.5)	19234	3.1174	-7471B	-	PPB	06 Sep 2019 11:28:58	U	SMPL
K4694-19 - 1	T3-1-3-(0-1.5)	5603	0.8526	-7471B	-	PPB	06 Sep 2019 11:31:15	U	SMPL
K4695-06 - 1	T5-1-4-(0-2.5)	8000	1.2509	-7471B	-	PPB	06 Sep 2019 11:33:33	U	SMPL
PB122858BL - 1	PBS	192	-0.0464	-7471B	-	PPB	06 Sep 2019 11:35:49	U	SMPL
CCV81 - 1	CCV81	30817	5.0418	-7471B	-	PPB	06 Sep 2019 11:38:05	U	SMPL
CCB81 - 1	CCB81	164	-0.0511	-7471B	-	PPB	06 Sep 2019 11:40:22	U	SMPL
PB122858BS - 1	LCSS	23366	3.8039	-7471B	-	PPB	06 Sep 2019 11:42:38	U	SMPL
K4656-01 - 1	AU-06-090519	13766	2.2089	-7471B	-	PPB	06 Sep 2019 11:44:55	U	SMPL
K4656-01DUP - 1	AU-06-090519DUP	13799	2.2144	-7471B	-	PPB	06 Sep 2019 11:47:11	U	SMPL
K4656-01MS - 1	AU-06-090519MS	35891	5.8849	-7471B	-	PPB	06 Sep 2019 11:49:27	U	SMPL
K4656-01MSD - 1	AU-06-090519MSD	35224	5.7740	-7471B	-	PPB	06 Sep 2019 11:51:44	U	SMPL
K4661-01 - 1	HD-01-090519	3475	0.4991	-7471B	-	PPB	06 Sep 2019 11:54:01	U	SMPL
K4663-01 - 1	OK-03-090519	553688	HIGH	-7471B	-	PPB	06 Sep 2019 11:56:19	X	
K4669-01 - 1	TR-05-090519	3925	0.5738	-7471B	-	PPB	06 Sep 2019 11:58:11	U	SMPL
K4693-03 - 1	TP-18-S	2145	0.2781	-7471B	-	PPB	06 Sep 2019 12:00:30	U	SMPL
K4693-07 - 1	TP-18-D	1922	0.2410	-7471B	-	PPB	06 Sep 2019 12:02:46	U	SMPL
CCV82 - 1	CCV82	30438	4.9789	-7471B	-	PPB	06 Sep 2019 12:07:10	U	SMPL
CCB82 - 1	CCB82	178	-0.0487	-7471B	-	PPB	06 Sep 2019 12:09:26	U	SMPL
K4716-03 - 1	TP-20-S	2512	0.3391	-7471B	-	PPB	06 Sep 2019 12:11:43	U	SMPL
K4716-07 - 1	TP-20-D	1053	0.0966	-7471B	-	PPB	06 Sep 2019 12:13:59	U	SMPL
K4683-01LX5 - 1		31501	5.1555	-7471B	-	PPB	06 Sep 2019 12:16:15	U	SMPL
K4683-01A - 1		174108	28.8492	-7471B	-	PPB	06 Sep 2019 12:18:32	U	SMPL
K4656-01LX5 - 1		2717	0.3731	-7471B	-	PPB	06 Sep 2019 12:20:48	U	SMPL
K4656-01A - 1		39687	6.5156	-7471B	-	PPB	06 Sep 2019 12:23:07	U	SMPL
K4650-15DLX3 - 1		28691	4.6886	-7471B	-	PPB	06 Sep 2019 12:25:24	U	SMPL
K4683-01DLX5 - 1		31487	5.1532	-7471B	-	PPB	06 Sep 2019 12:27:42	U	SMPL
K4683-01DUPDLX5 - 1		32176	5.2676	-7471B	-	PPB	06 Sep 2019 12:30:00	U	SMPL
K4683-01MSDLX5 - 1		35793	5.8686	-7471B	-	PPB	06 Sep 2019 12:32:18	U	SMPL
CCV83 - 1	CCV83	30190	4.9377	-7471B	-	PPB	06 Sep 2019 12:34:35	U	SMPL
CCB83 - 1	CCB83	148	-0.0537	-7471B	-	PPB	06 Sep 2019 12:36:52	U	SMPL
K4683-01MSDDLX5 - 1		34943	5.7274	-7471B	-	PPB	06 Sep 2019 12:39:08	U	SMPL
K4683-01DL2X25 - 1		6286	0.9661	-7471B	-	PPB	06 Sep 2019 12:41:25	U	SMPL
K4683-01ADLX5 - 1		35978	5.8993	-7471B	-	PPB	06 Sep 2019 12:48:03	U	SMPL
K4683-03DLX3 - 1		25051	4.0838	-7471B	-	PPB	06 Sep 2019 12:50:19	U	SMPL
K4683-04DLX3 - 1		28507	4.6580	-7471B	-	PPB	06 Sep 2019 12:52:36	U	SMPL
K4663-01DLX10 - 1		90511	14.9598	-7471B	-	PPB	06 Sep 2019 12:54:53	U	SMPL
K4663-01DLX50 - 1		17344	2.8033	-7471B	-	PPB	06 Sep 2019 13:08:37	U	SMPL
CCV84 - 1	CCV84	30458	4.9822	-7471B	-	PPB	06 Sep 2019 13:10:54	U	SMPL
CCB84 - 1	CCB84	163	-0.0512	-7471B	-	PPB	06 Sep 2019 13:13:12	U	SMPL