


LB105089

7470A

INSTRUMENT ID: CV1

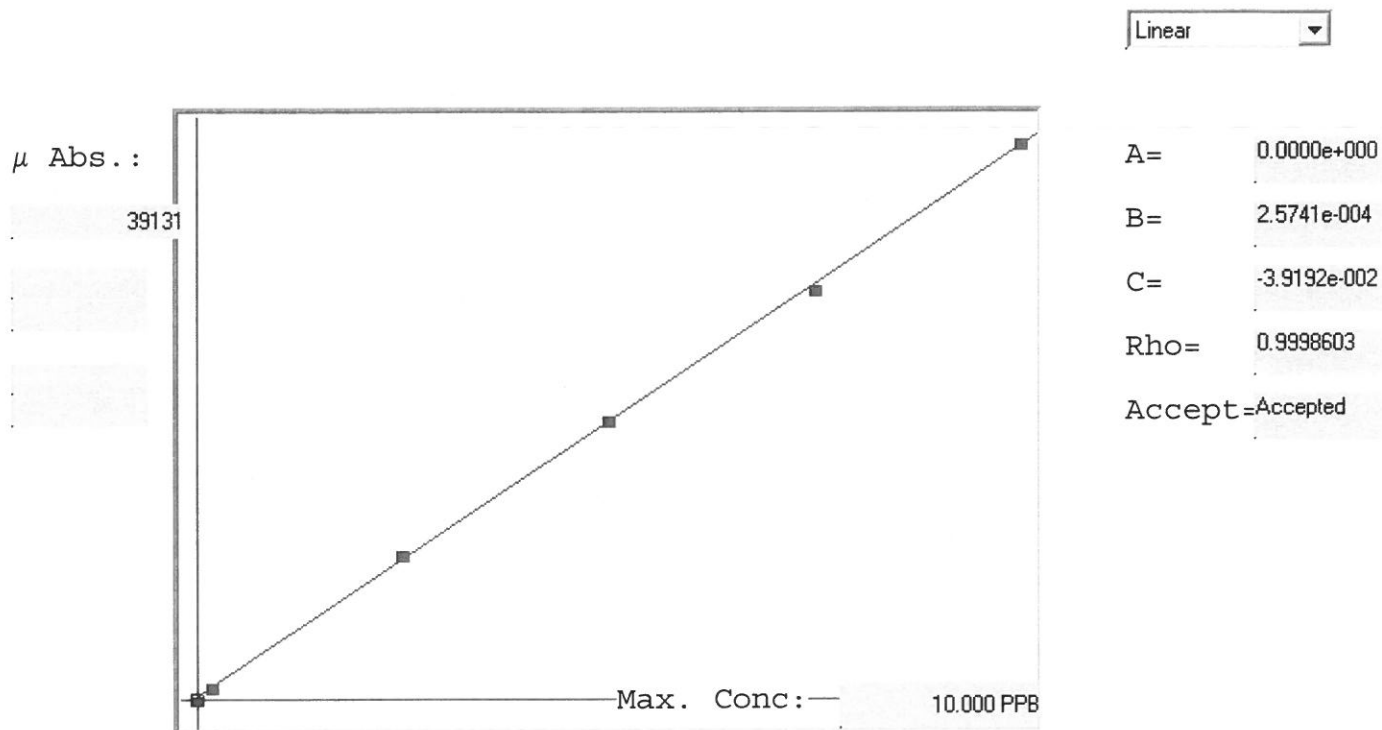

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.030	-0.030	37	0.000	37				
0.2	0.200	0.173	-0.027	824	0.0 %	824				
2.5	2.500	2.582	0.082	10182	0.0 %	10182				
5.0	5.000	5.047	0.047	19760	0.0 %	19760				
7.5	7.500	7.394	-0.106	28878	0.0 %	28878				
10.0	10.000	10.034	0.034	39131	0.0 %	39131				

LB105089 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 12 Sep 2019 10:35:10				
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
0.0 - 1	50.0	37	-	0.0000	7470A	PPB	12 Sep 2019 10:40:40	S Std
0.2 - 1	50.2	824	-	0.2000	7470A	PPB	12 Sep 2019 10:42:49	S Std
2.5 - 1	52.5	10182	-	2.5000	7470A	PPB	12 Sep 2019 10:44:58	S Std
5.0 - 1	55.0	19760	-	5.0000	7470A	PPB	12 Sep 2019 10:47:07	S Std
7.5 - 1	57.5	28878	-	7.5000	7470A	PPB	12 Sep 2019 10:49:16	S Std
10.0 - 1	510.0	39131	-	10.0000	7470A	PPB	12 Sep 2019 10:51:25	S Std
ICV09 - 1	ICV09	16140	4.1154	-	7470A	PPB	12 Sep 2019 10:54:00	U SMPL
ICB09 - 1	ICB09	-32	-0.0474	-	7470A	PPB	12 Sep 2019 10:56:05	U SMPL
CCV12 - 1	CCV12	19285	4.9250	-	7470A	PPB	12 Sep 2019 10:58:12	U SMPL
CCB12 - 1	CCB12	5	-0.0379	-	7470A	PPB	12 Sep 2019 11:00:19	U SMPL
CRA - 1	CRA	840	0.1770	-	7470A	PPB	12 Sep 2019 11:02:26	U SMPL
HighStd - 1	HighStd	39473	10.1215	-	7470A	PPB	12 Sep 2019 11:04:32	U SMPL
ChkStd - 1	ChkStd	26260	6.7204	-	7470A	PPB	12 Sep 2019 11:06:39	U SMPL
PB123021BL - 1	PBW	358	0.0530	-	7470A	PPB	12 Sep 2019 11:08:47	U SMPL
PB123021BS - 1	LCSW	16034	4.0881	-	7470A	PPB	12 Sep 2019 11:10:54	U SMPL
K4650-14 - 1	TP-7	10	-0.0366	-	7470A	PPB	12 Sep 2019 11:13:03	U SMPL
K4650-16 - 1	TP-8	76	-0.0196	-	7470A	PPB	12 Sep 2019 11:15:10	U SMPL
K4806-02 - 1	DRUM-COMP	526	0.0962	-	7470A	PPB	12 Sep 2019 11:17:19	U SMPL
K4814-04 - 1	WC-1	184	0.0082	-	7470A	PPB	12 Sep 2019 11:19:28	U SMPL
CCV13 - 1	CCV13	19258	4.9180	-	7470A	PPB	12 Sep 2019 11:23:42	U SMPL
CCB13 - 1	CCB13	99	-0.0137	-	7470A	PPB	12 Sep 2019 11:25:48	U SMPL
K4814-06 - 1	WC-3	268	0.0298	-	7470A	PPB	12 Sep 2019 11:27:55	U SMPL
K4819-04 - 1	TP-2-S(1-4)	73	-0.0204	-	7470A	PPB	12 Sep 2019 11:30:02	U SMPL
K4819-08 - 1	TP-7-S(2-4)	62	-0.0232	-	7470A	PPB	12 Sep 2019 11:32:09	U SMPL
K4819-12 - 1	TP-7-D(4-10)	53	-0.0255	-	7470A	PPB	12 Sep 2019 11:34:17	U SMPL
K4819-12DUP - 1	TP-7-D(4-10)DUP	41	-0.0286	-	7470A	PPB	12 Sep 2019 11:36:26	U SMPL
K4819-12MS - 1	TP-7-D(4-10)MS	15570	3.9687	-	7470A	PPB	12 Sep 2019 11:38:34	U SMPL
K4819-12MSD - 1	TP-7-D(4-10)MSD	16196	4.1298	-	7470A	PPB	12 Sep 2019 11:40:43	U SMPL
PB123022BL - 1	PBW	421	0.0692	-	7470A	PPB	12 Sep 2019 11:42:51	U SMPL
PB123022BS - 1	LCSW	16390	4.1798	-	7470A	PPB	12 Sep 2019 11:45:00	U SMPL
K4790-02 - 1	DRUM-1	39	-0.0292	-	7470A	PPB	12 Sep 2019 11:47:07	U SMPL
CCV14 - 1	CCV14	19628	5.0132	-	7470A	PPB	12 Sep 2019 11:49:13	U SMPL
CCB14 - 1	CCB14	414	0.0674	-	7470A	PPB	12 Sep 2019 11:51:20	U SMPL
K4790-02DUP - 1	DRUM-1DUP	46	-0.0274	-	7470A	PPB	12 Sep 2019 11:53:27	U SMPL
K4790-02MS - 1	DRUM-1MS	15614	3.9800	-	7470A	PPB	12 Sep 2019 11:55:34	U SMPL
K4790-02MSD - 1	DRUM-1MSD	15985	4.0755	-	7470A	PPB	12 Sep 2019 11:57:40	U SMPL
PB123021TB - 1	PB122979TB	43	-0.0281	-	7470A	PPB	12 Sep 2019 11:59:48	U SMPL
PB123022TB - 1	PB122981TB	58	-0.0243	-	7470A	PPB	12 Sep 2019 12:01:55	U SMPL
K4819-12LX5 - 1		130	-0.0057	-	7470A	PPB	12 Sep 2019 12:04:02	U SMPL
K4819-12A - 1		16228	4.1381	-	7470A	PPB	12 Sep 2019 12:06:11	U SMPL
K4790-02LX5 - 1		5	-0.0379	-	7470A	PPB	12 Sep 2019 12:08:23	U SMPL
K4790-02A - 1		15645	3.9880	-	7470A	PPB	12 Sep 2019 12:10:34	U SMPL
K4814-05 - 1	WC-2	769	0.1588	-	7470A	PPB	12 Sep 2019 12:12:41	U SMPL
CCV15 - 1	CCV15	19426	4.9612	-	7470A	PPB	12 Sep 2019 12:14:48	U SMPL
CCB15 - 1	CCB15	44	-0.0279	-	7470A	PPB	12 Sep 2019 12:16:56	U SMPL