

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : CT

Instrument ID : Konelab

9/18/2019 16:27

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.568	0.0	0.090	
ICB1	-0.252	0.0	0.001	
CCV1	248.035	0.0	0.227	
CCB1	-0.302	0.0	0.001	
PB123171BL	-0.252	0.0	0.001	
PB123171BS	98.994	0.0	0.091	
MIDPB123171	250.284	0.0	0.229	
K4843-23	551.508	0.0	0.502	Test limit high
K4843-23DLX2	274.525	0.0	0.251	
CCV2	251.083	0.0	0.229	
CCB2	0.004	0.0	0.002	

N	11
Mean	161.018
SD	173.4524
CV%	107.72

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : CT

Instrument ID : Konelab

9/18/2019 13:54


Test Total CN

Accepted 9/18/2019 13:46

Factor 1102
Bias 0.002

Coeff. of det. 0.999960

Errors

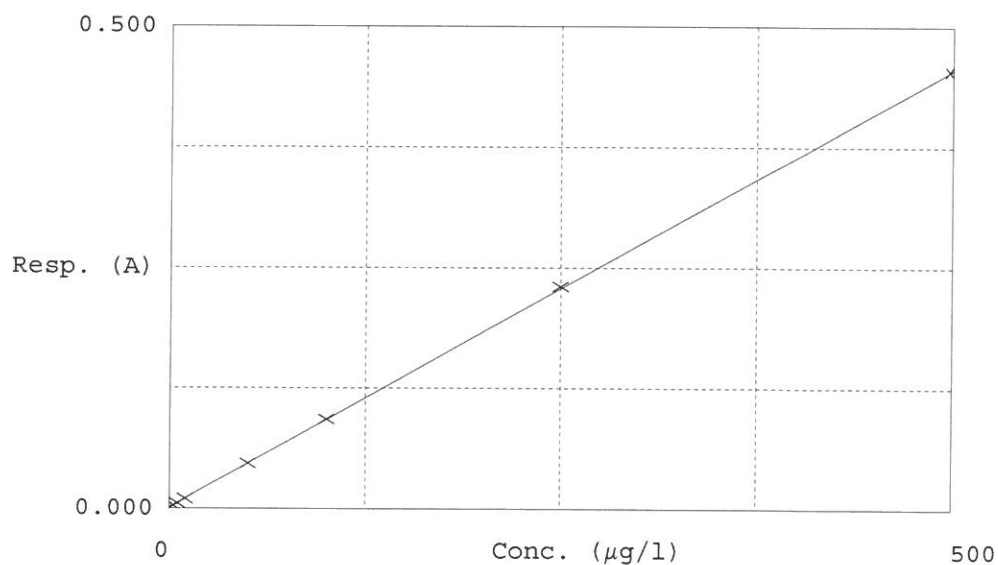

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.5188	0.0000	
2	5.0PPBCN	0.005	4.3631	5.0000	
3	10PPBCN	0.010	9.6687	10.0000	
4	50PPBCN	0.047	49.8540	50.0000	
5	100PPBCN	0.093	100.5325	100.0000	
6	250PPBCN	0.230	252.3589	250.0000	
7	500PPBCN	0.454	498.7417	500.0000	

9/18/19
CT

Aquakem v. 7.2AQ1

Results from time period:

Wed Sep 18 16:21:12 2019

Wed Sep 18 16:21:22 2019

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.5188	µg/l	9/18/2019 13:43:13	
5.OPPBCN	A	Total CN	P	4.3631	µg/l	9/18/2019 13:43:14	
10PPBCN	A	Total CN	P	9.6687	µg/l	9/18/2019 13:43:15	
50PPBCN	A	Total CN	P	49.854	µg/l	9/18/2019 13:43:16	
100PPBCN	A	Total CN	P	100.5325	µg/l	9/18/2019 13:43:17	
250PPBCN	A	Total CN	P	252.3589	µg/l	9/18/2019 13:43:18	
500PPBCN	A	Total CN	P	498.7417	µg/l	9/18/2019 13:43:19	
ICV1	S	Total CN	P	97.568	µg/l	9/18/2019 16:21:12	
ICB1	S	Total CN	P	-0.2516	µg/l	9/18/2019 16:21:13	
CCV1	S	Total CN	P	248.0348	µg/l	9/18/2019 16:21:14	
CCB1	S	Total CN	P	-0.3018	µg/l	9/18/2019 16:21:15	
PB123171BL	S	Total CN	P	-0.252	µg/l	9/18/2019 16:21:16	
PB123171BS	S	Total CN	P	98.9941	µg/l	9/18/2019 16:21:17	
MIDPB123171	S	Total CN	P	250.2839	µg/l	9/18/2019 16:21:18	
K4843-23	S	Total CN	P	551.5084	µg/l	9/18/2019 16:21:19	
K4843-23DLX2	S	Total CN	P	274.5251	µg/l	9/18/2019 16:21:20	
CCV2	S	Total CN	P	251.0834	µg/l	9/18/2019 16:21:21	
CCB2	S	Total CN	P	0.0035	µg/l	9/18/2019 16:21:22	